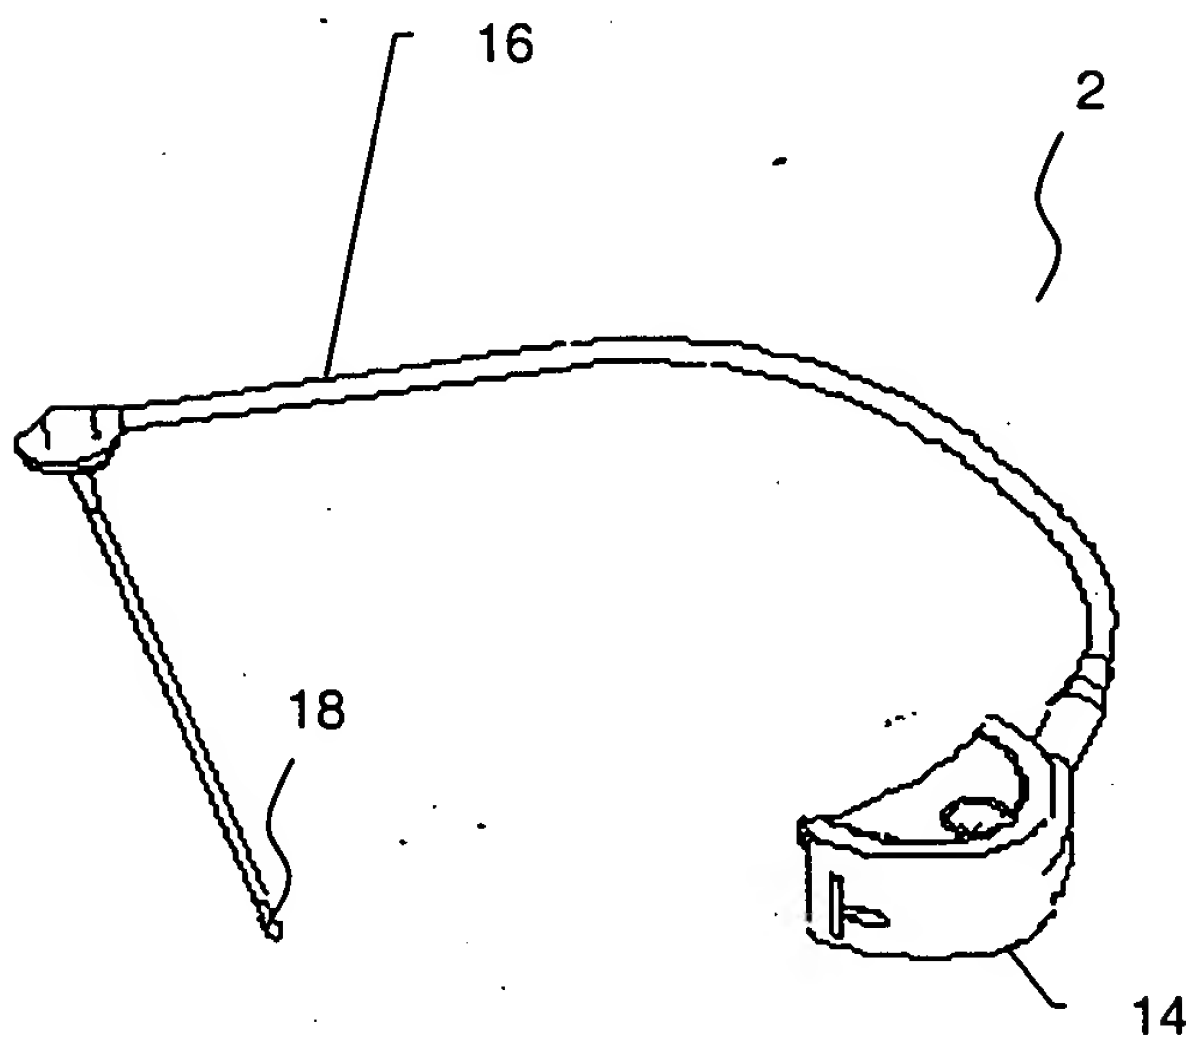


**FIGURE 1A**



**FIGURE 1B**

[illegible]

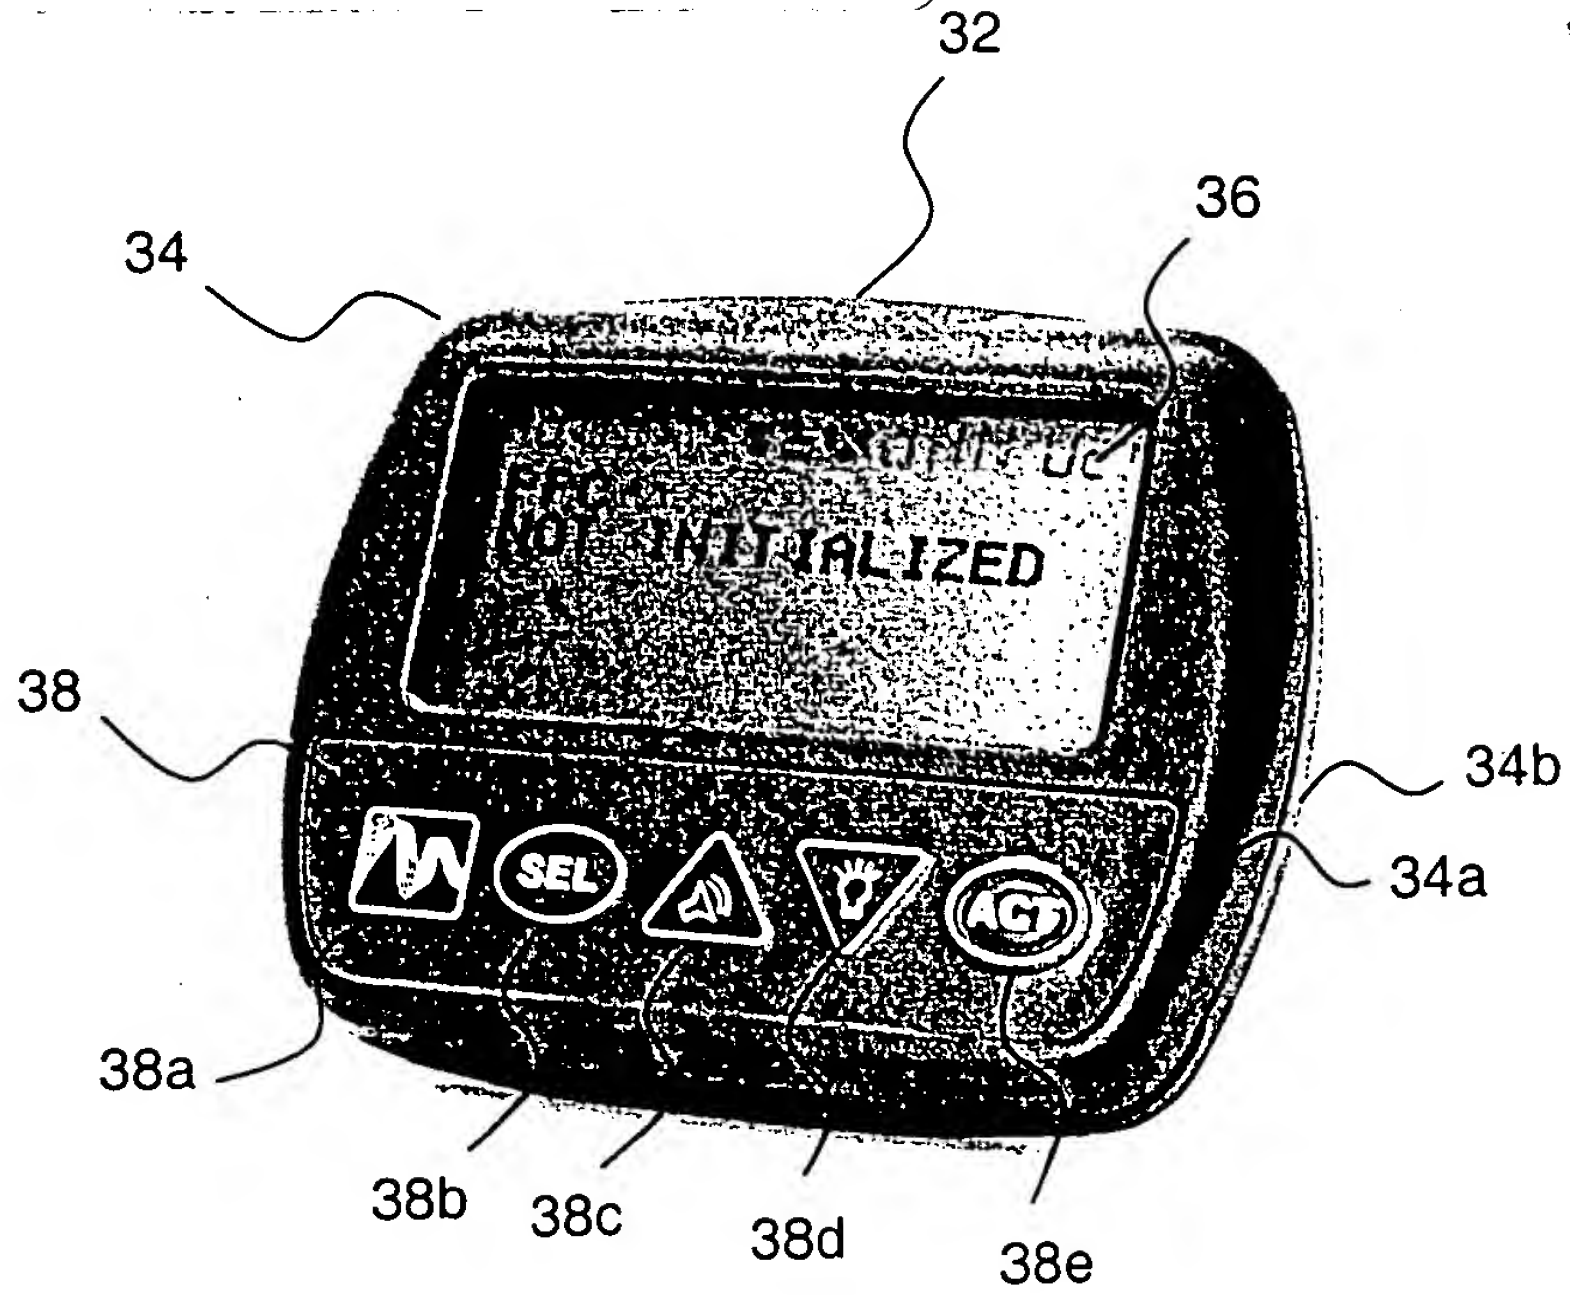


FIGURE 2

0975196-05001

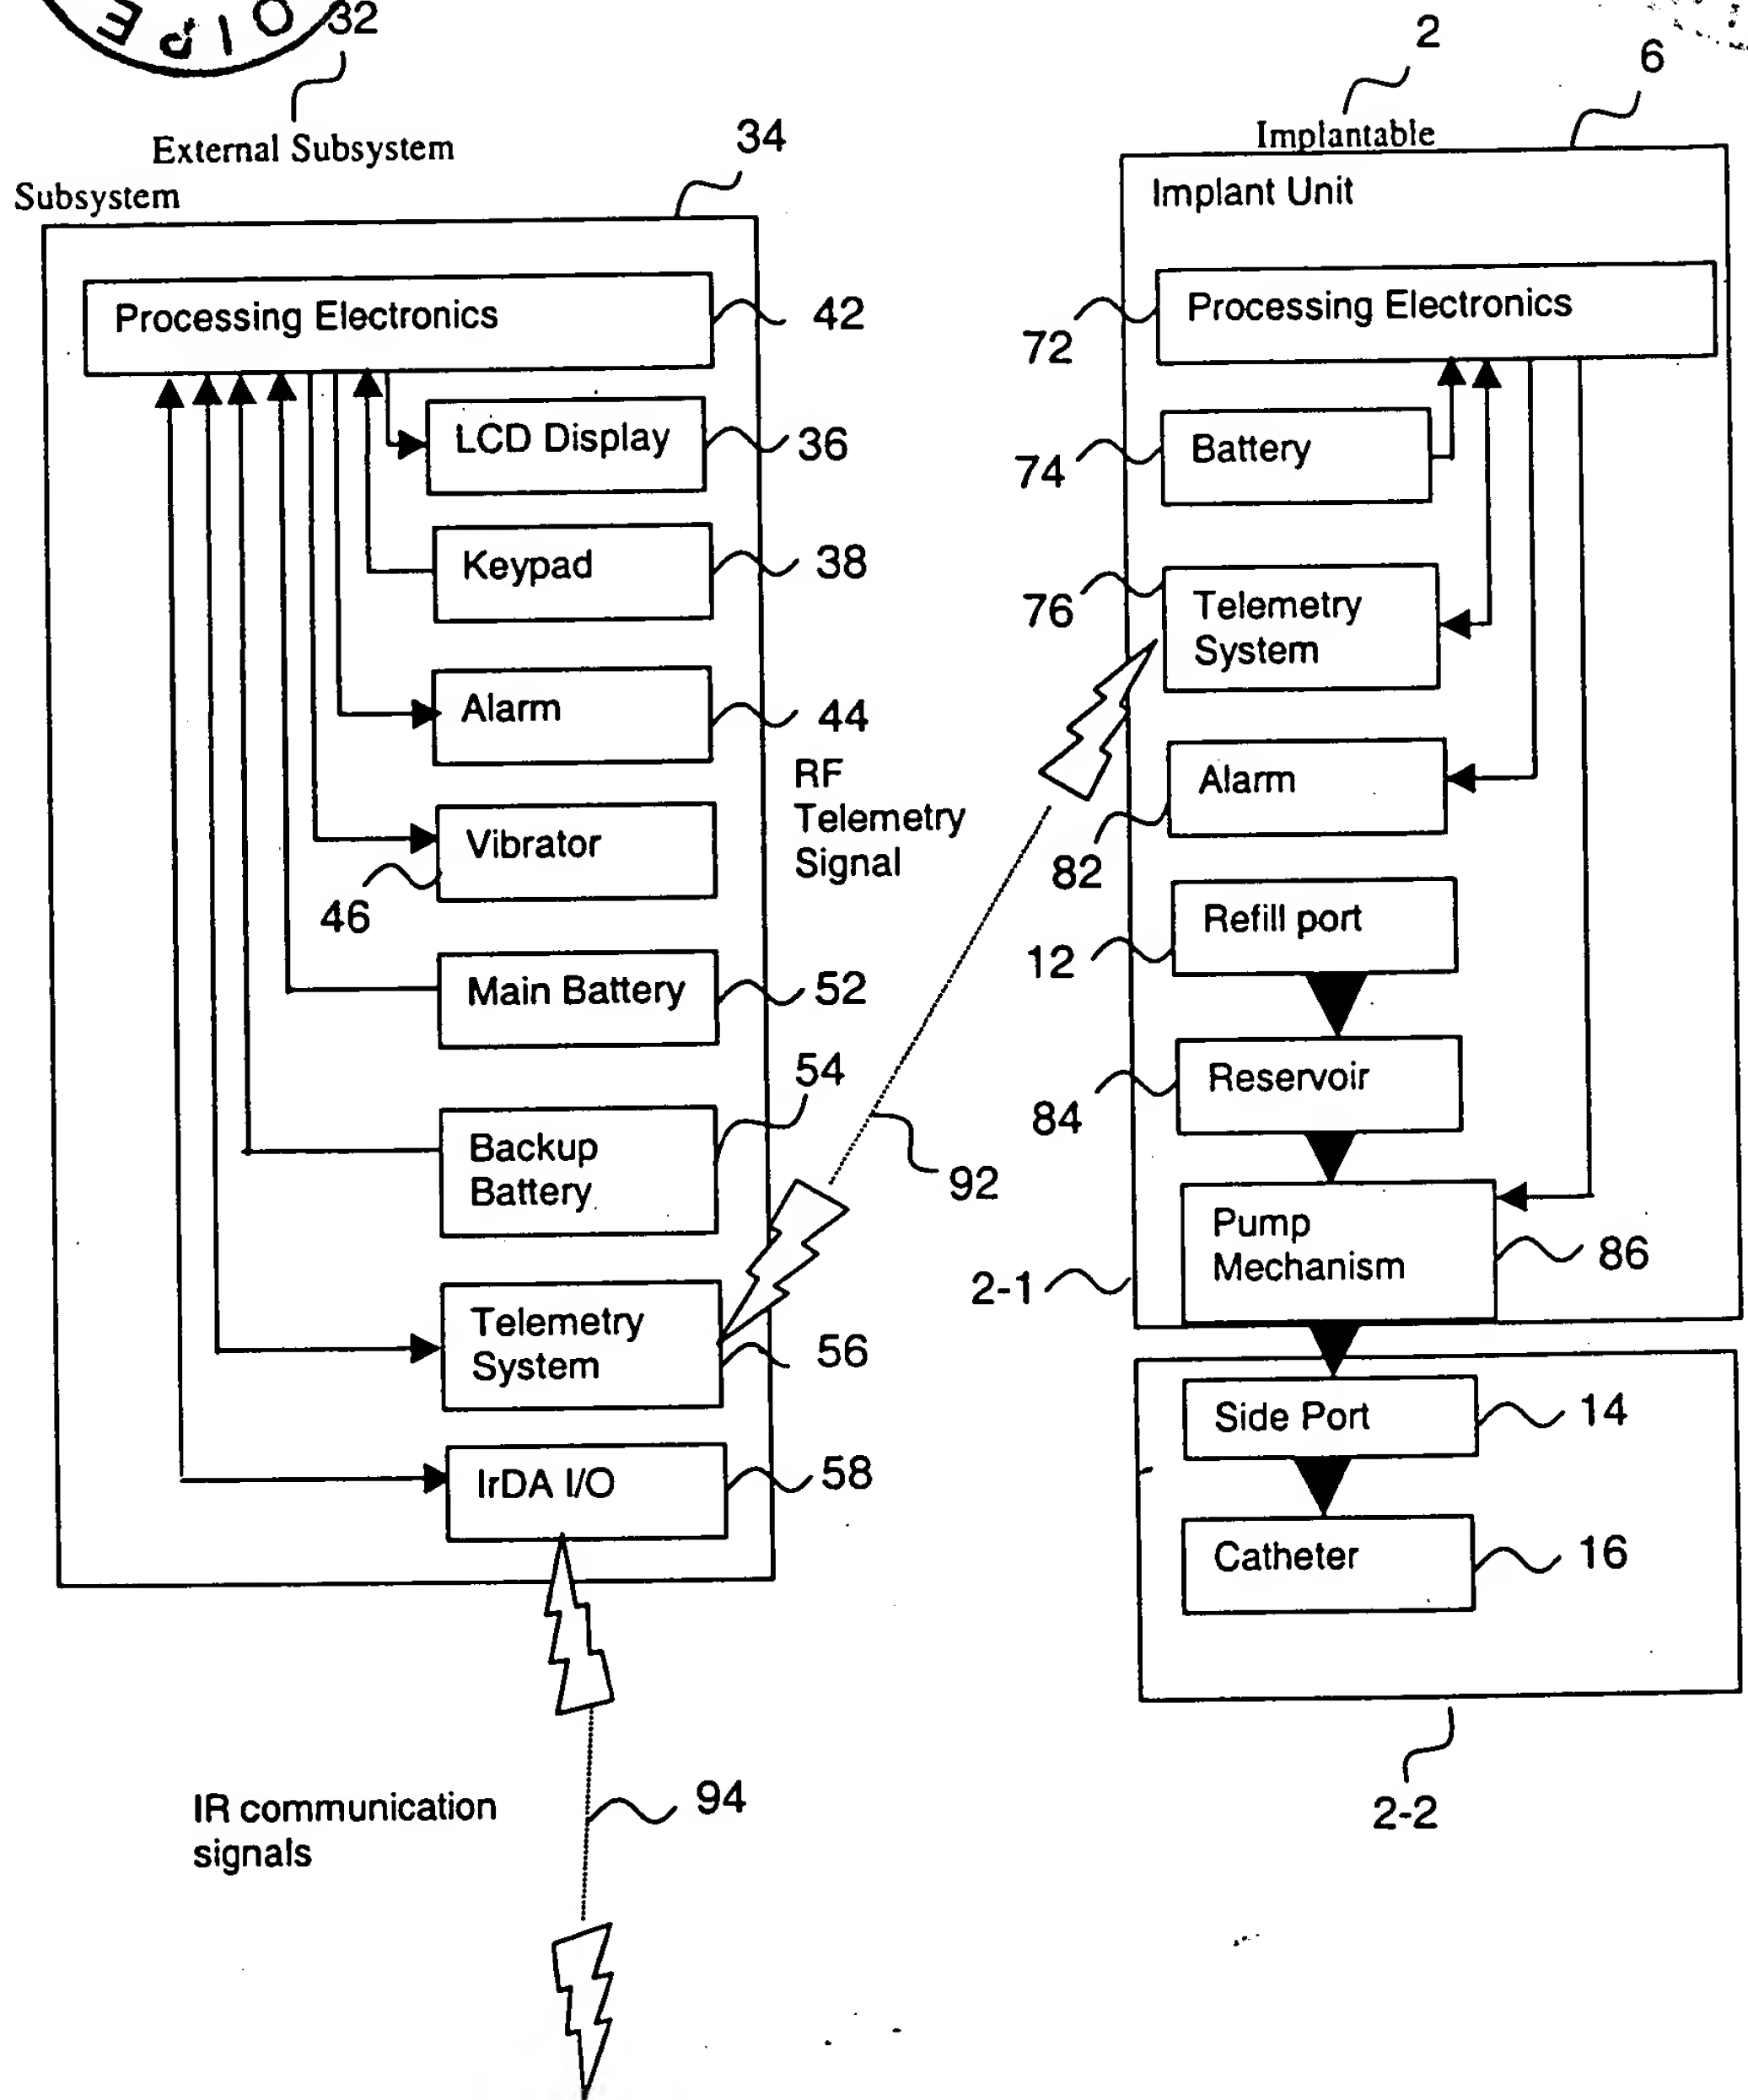
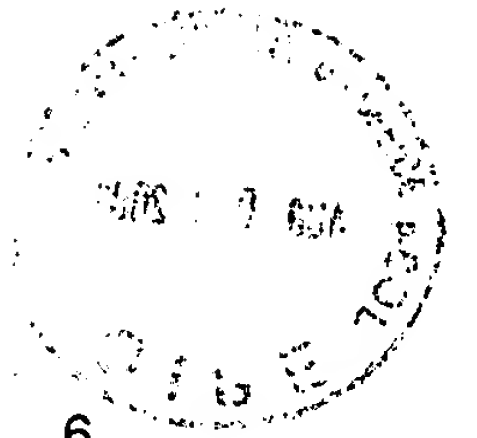


FIGURE 3

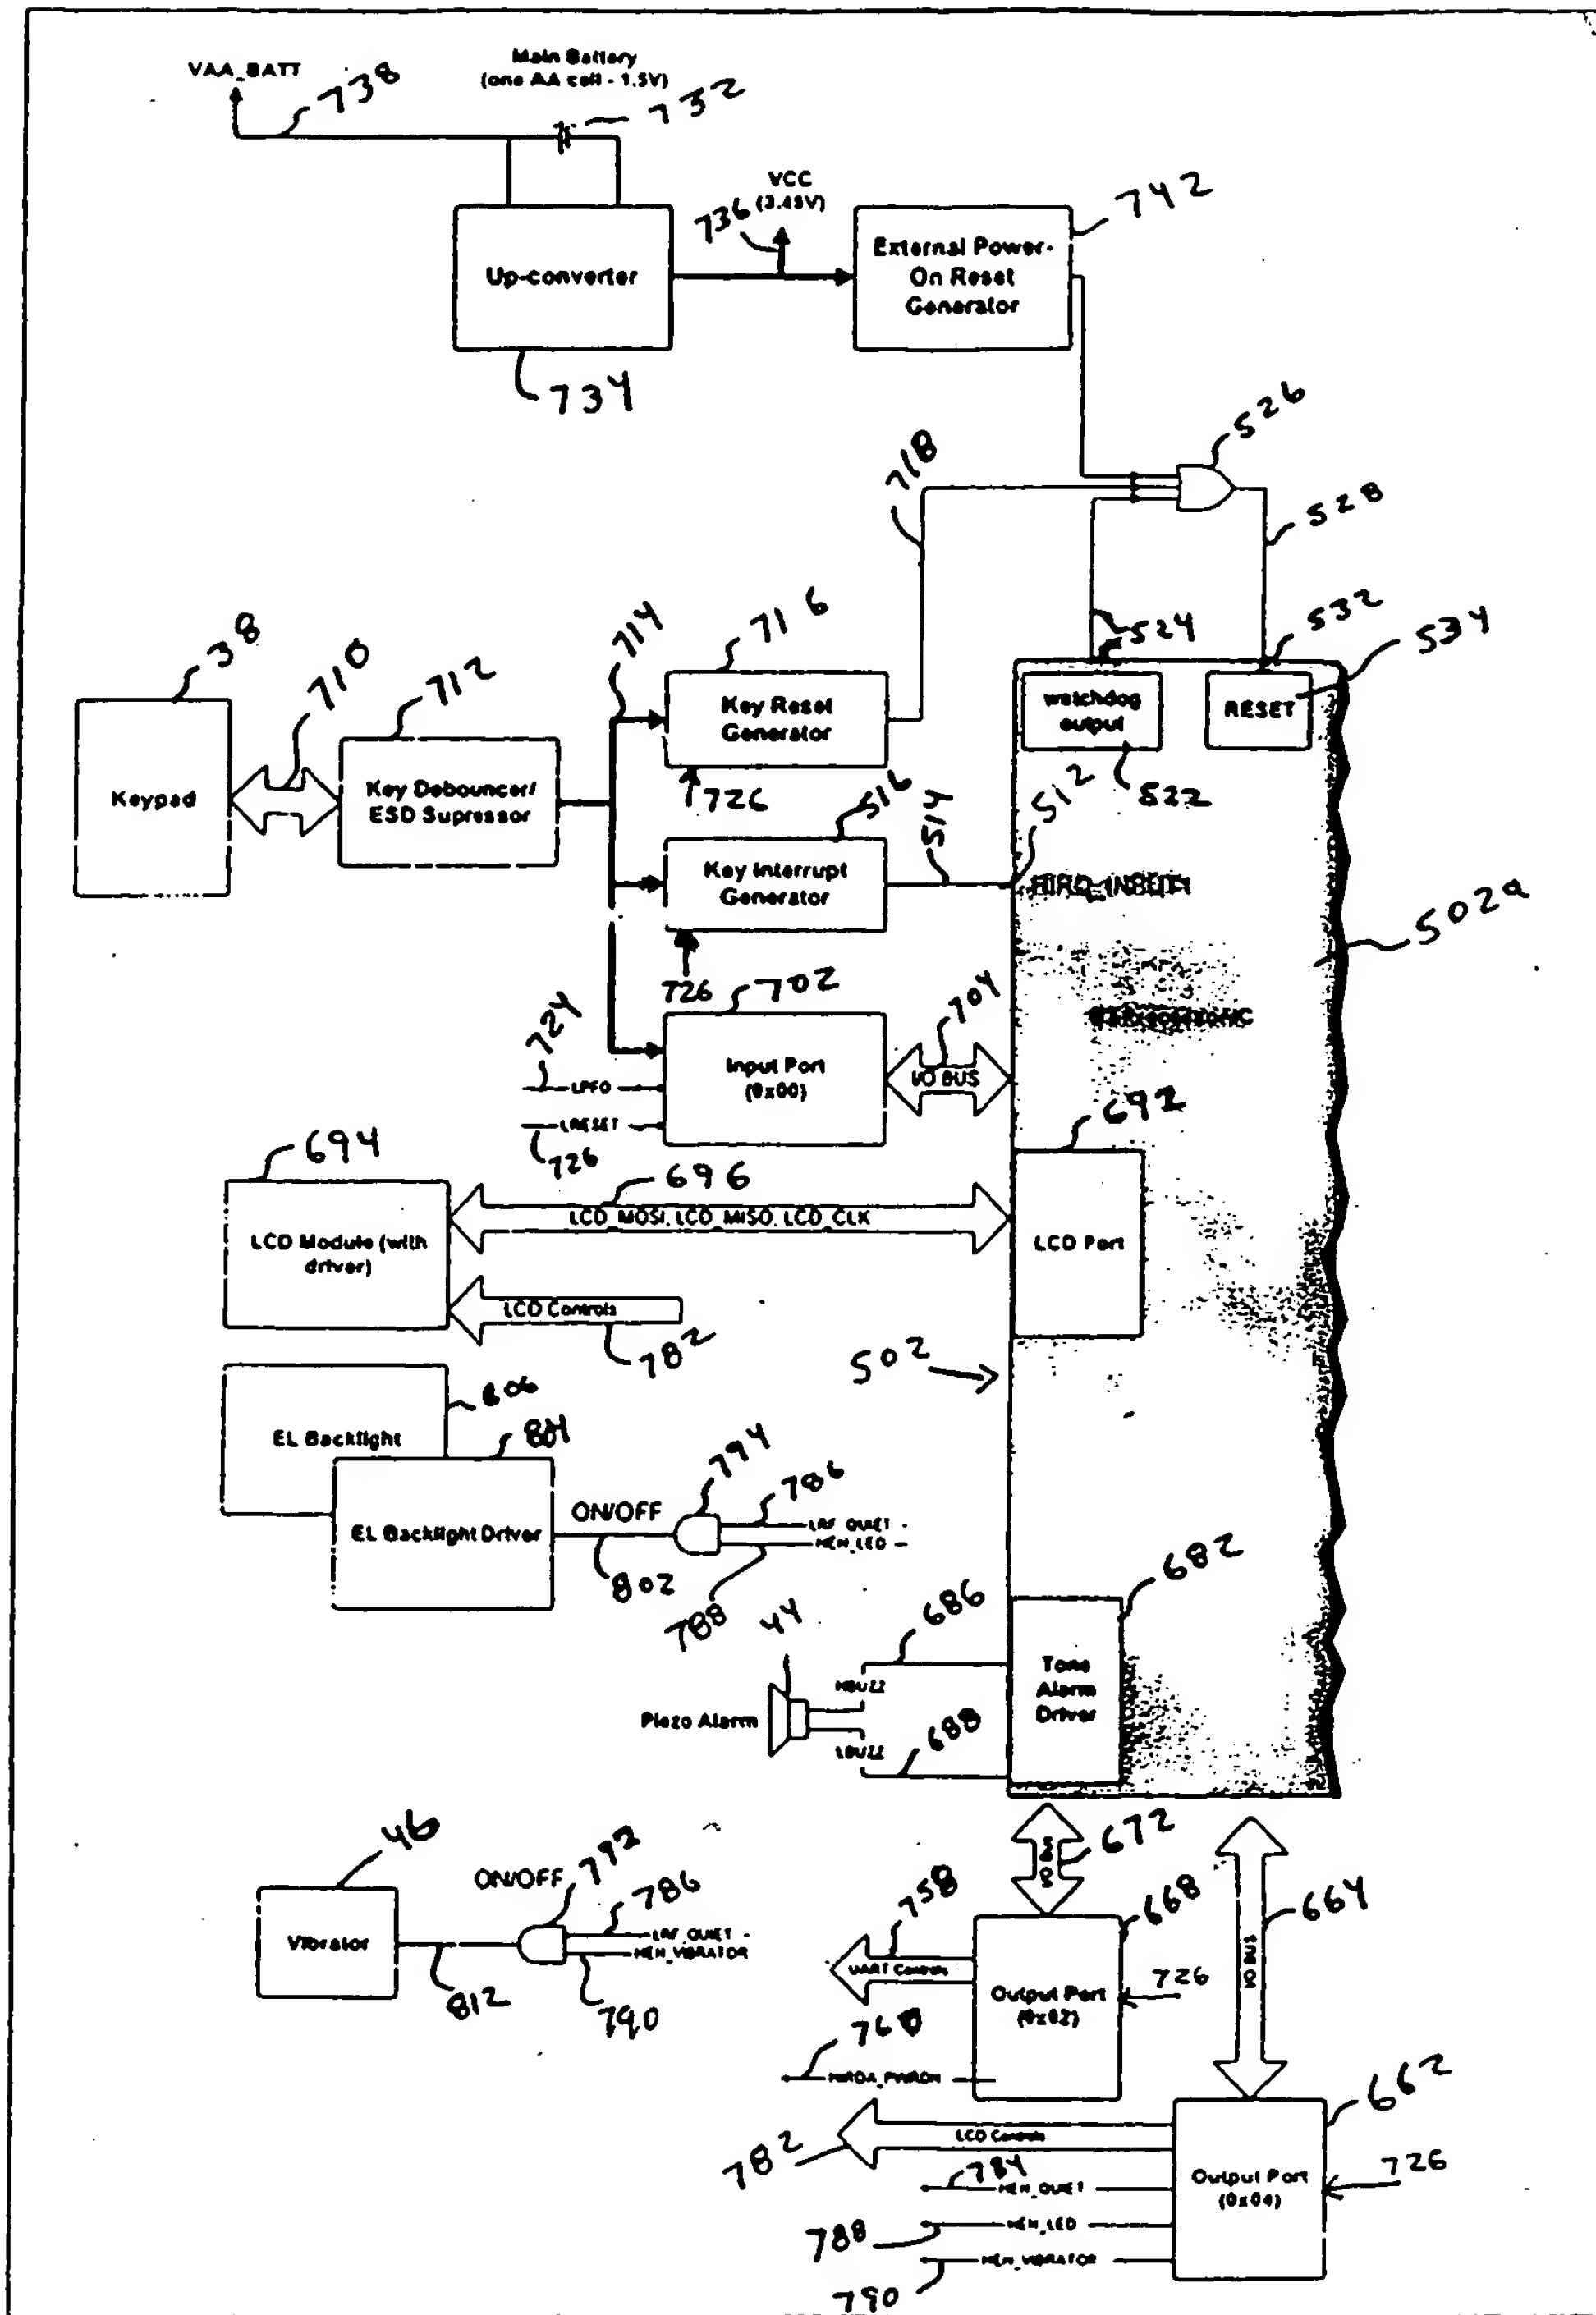


FIGURE 4a

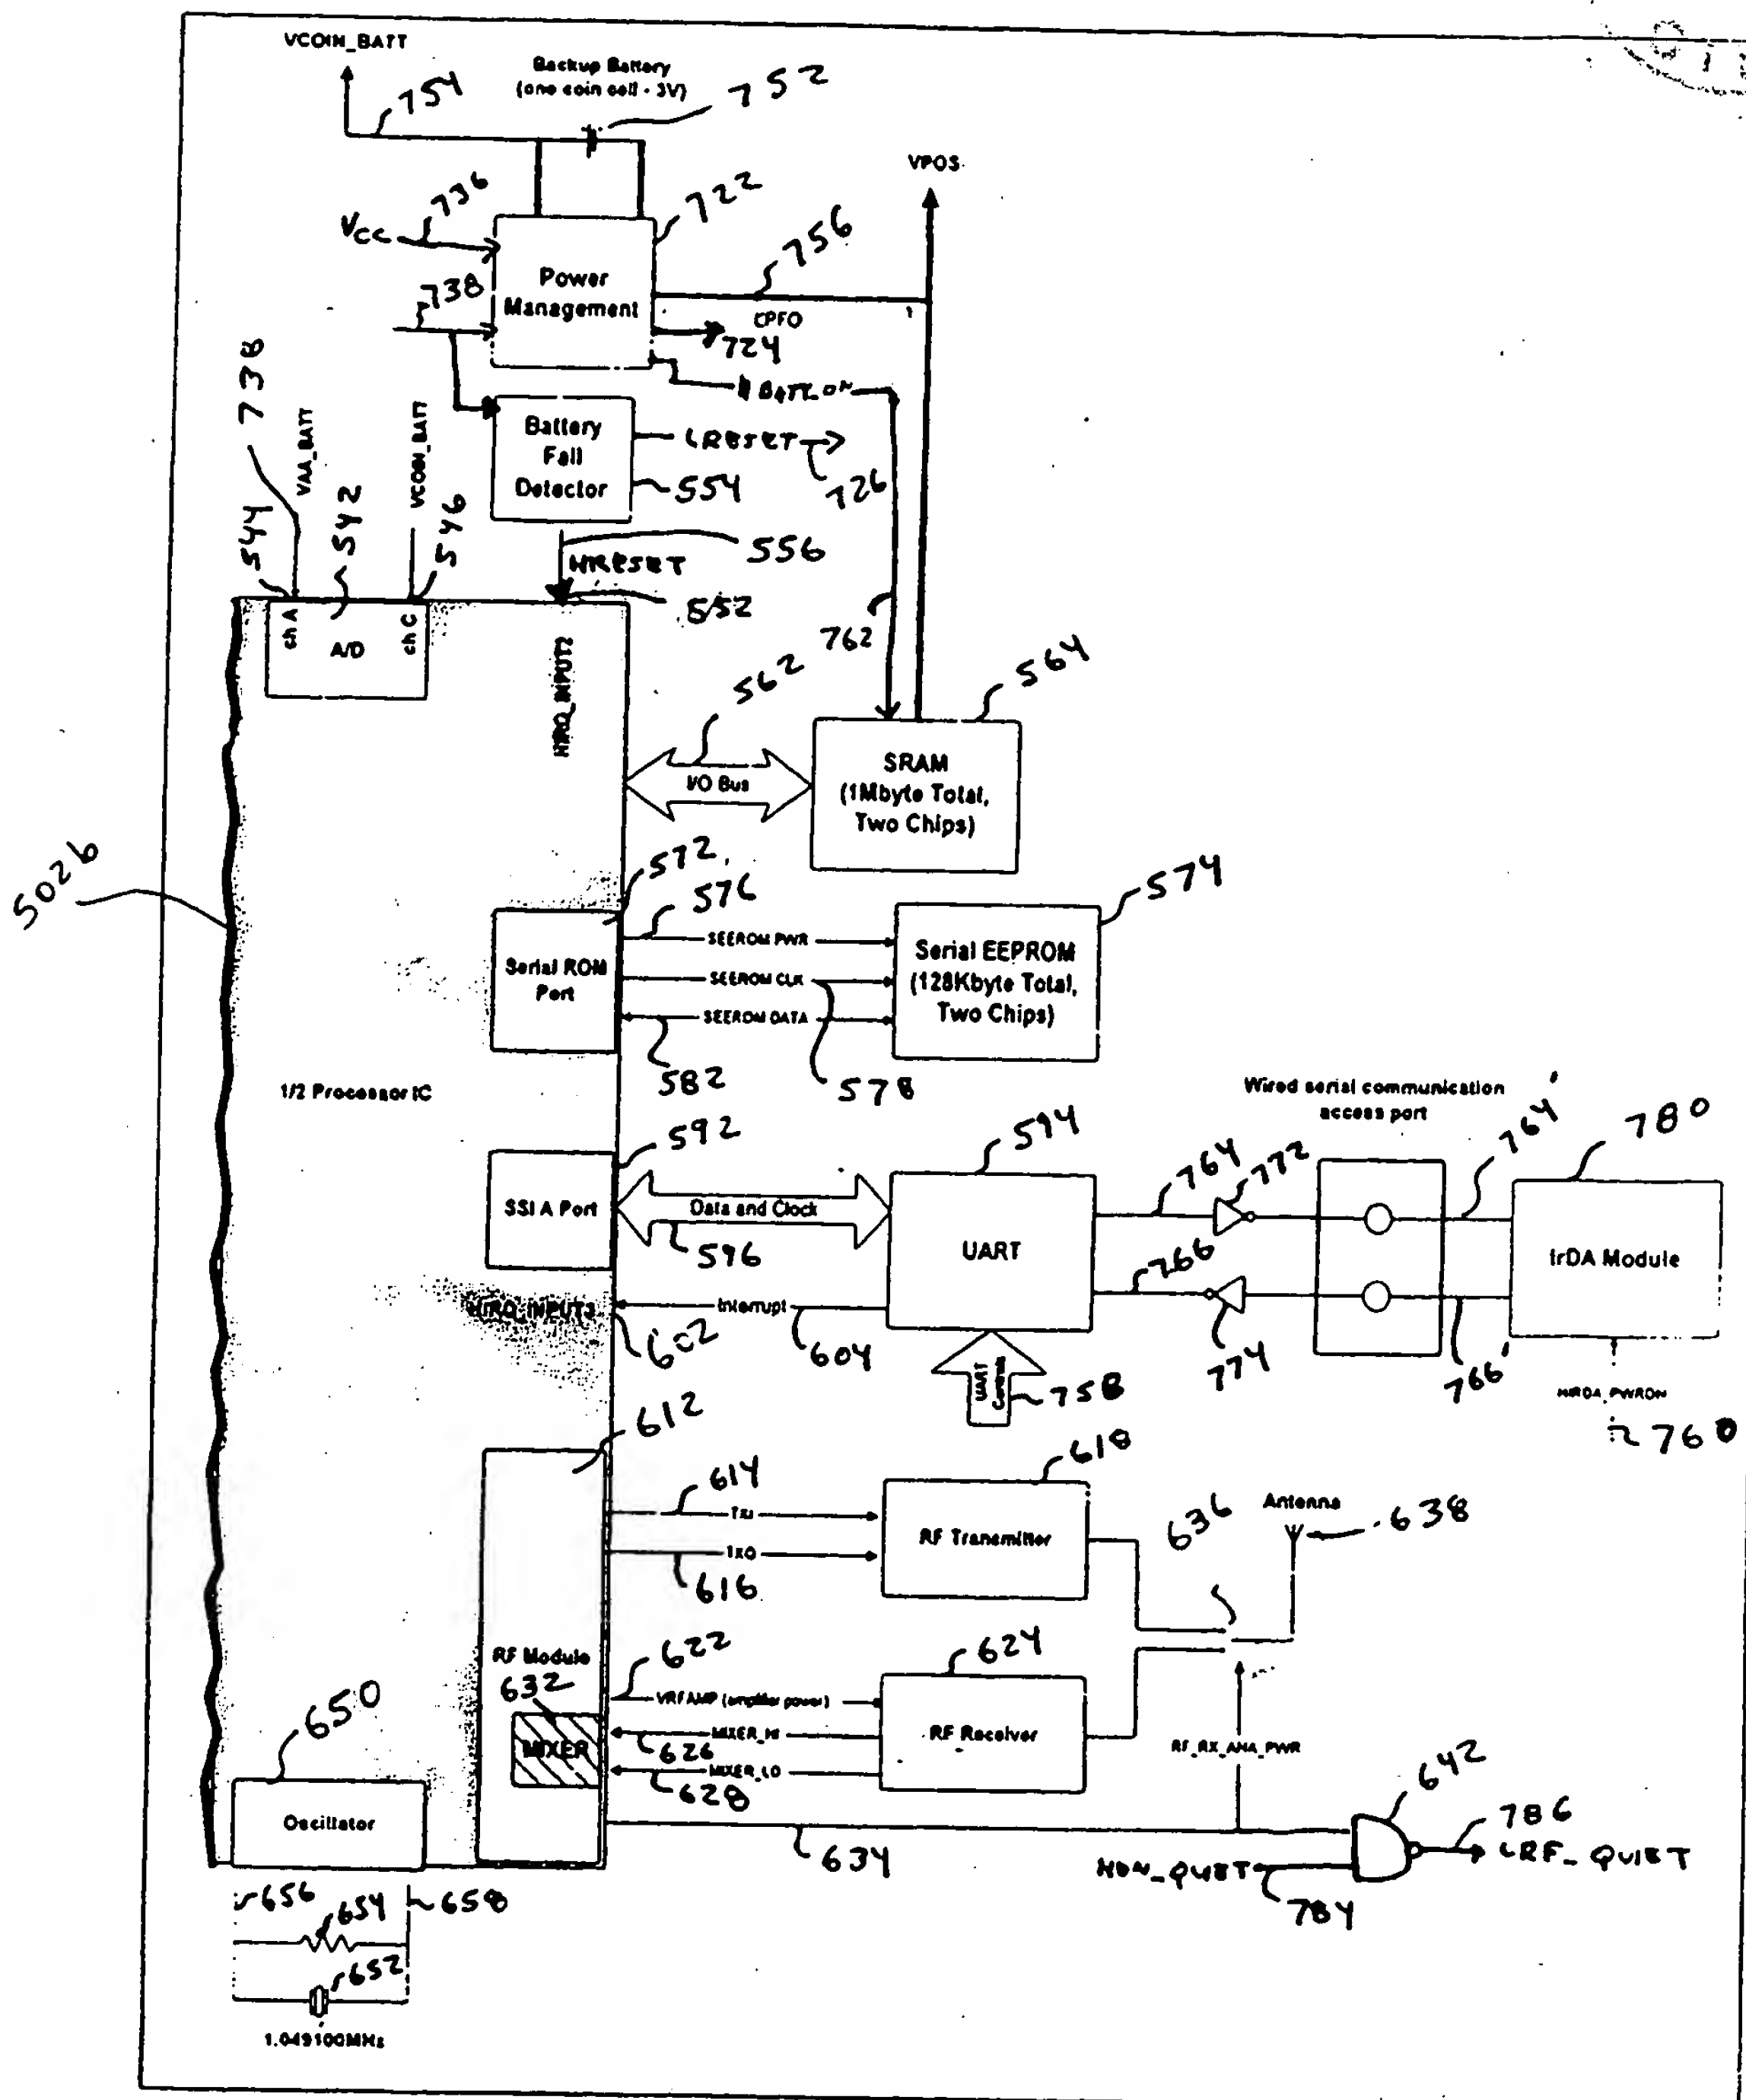


FIGURE 4b



- 88:88 → Time of Day
- ⌚ → Battery
- 🔊 → Alarm
- 📊 → Reservoir Volume Level
- ⊗ → Delivery (Bolus/Basal)
- 8888 → Month
- 88 → Date of Month

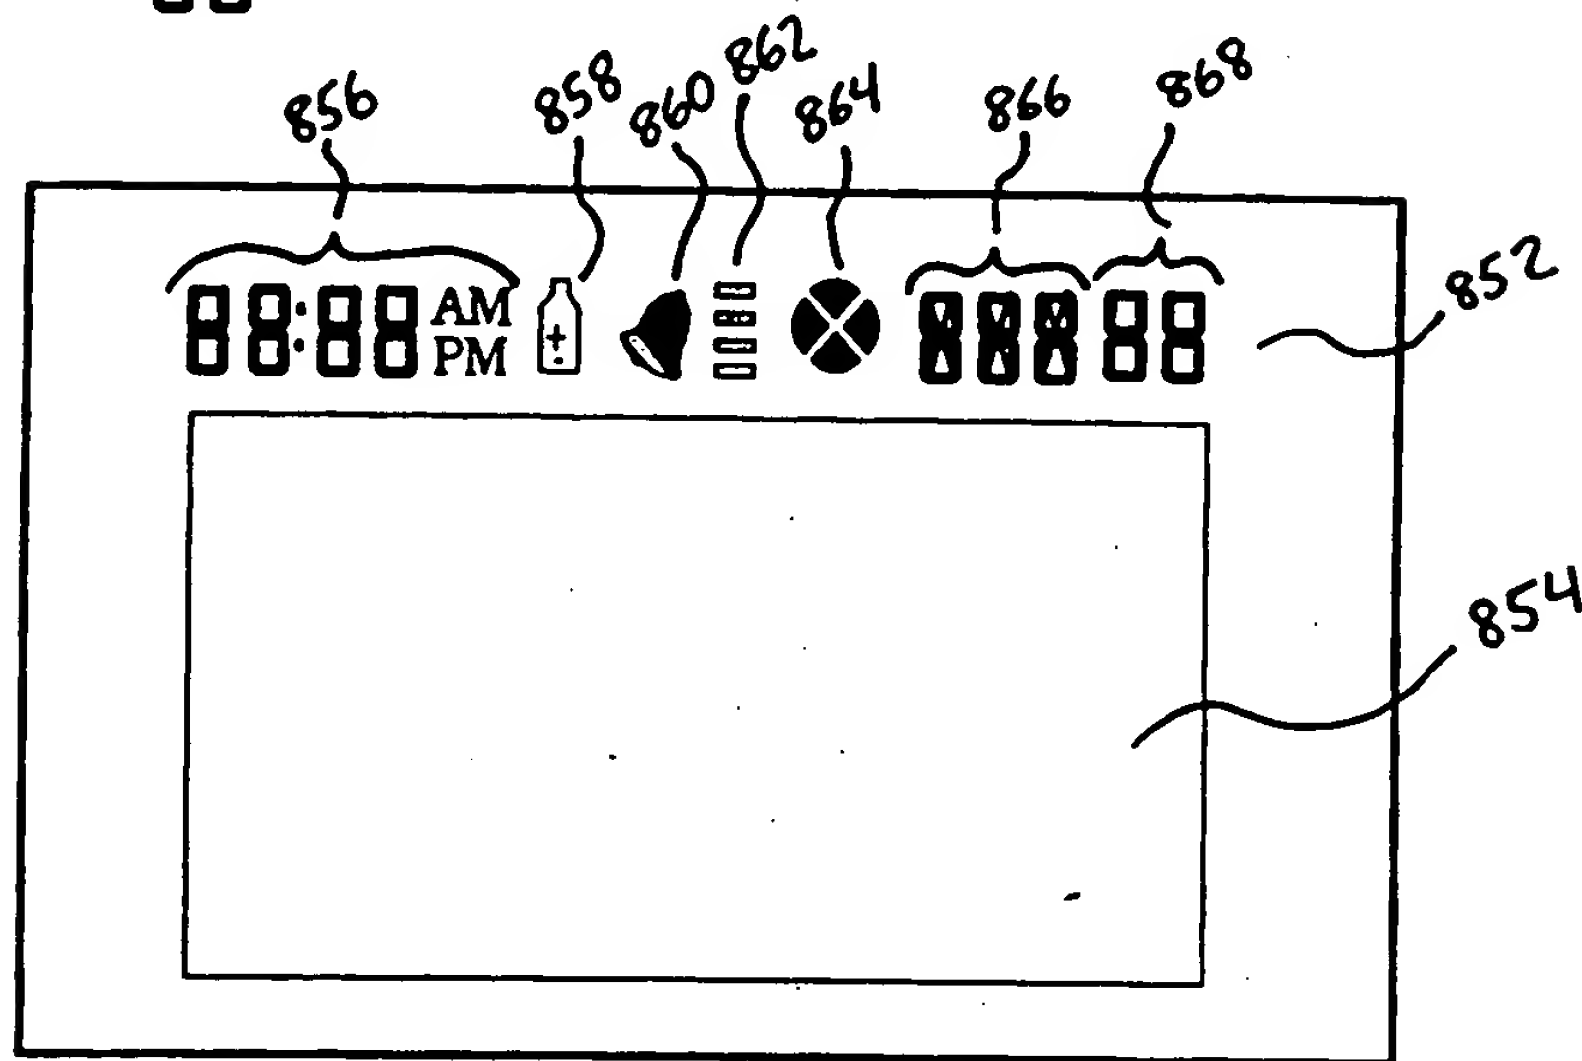


FIGURE 5

09768196-080501

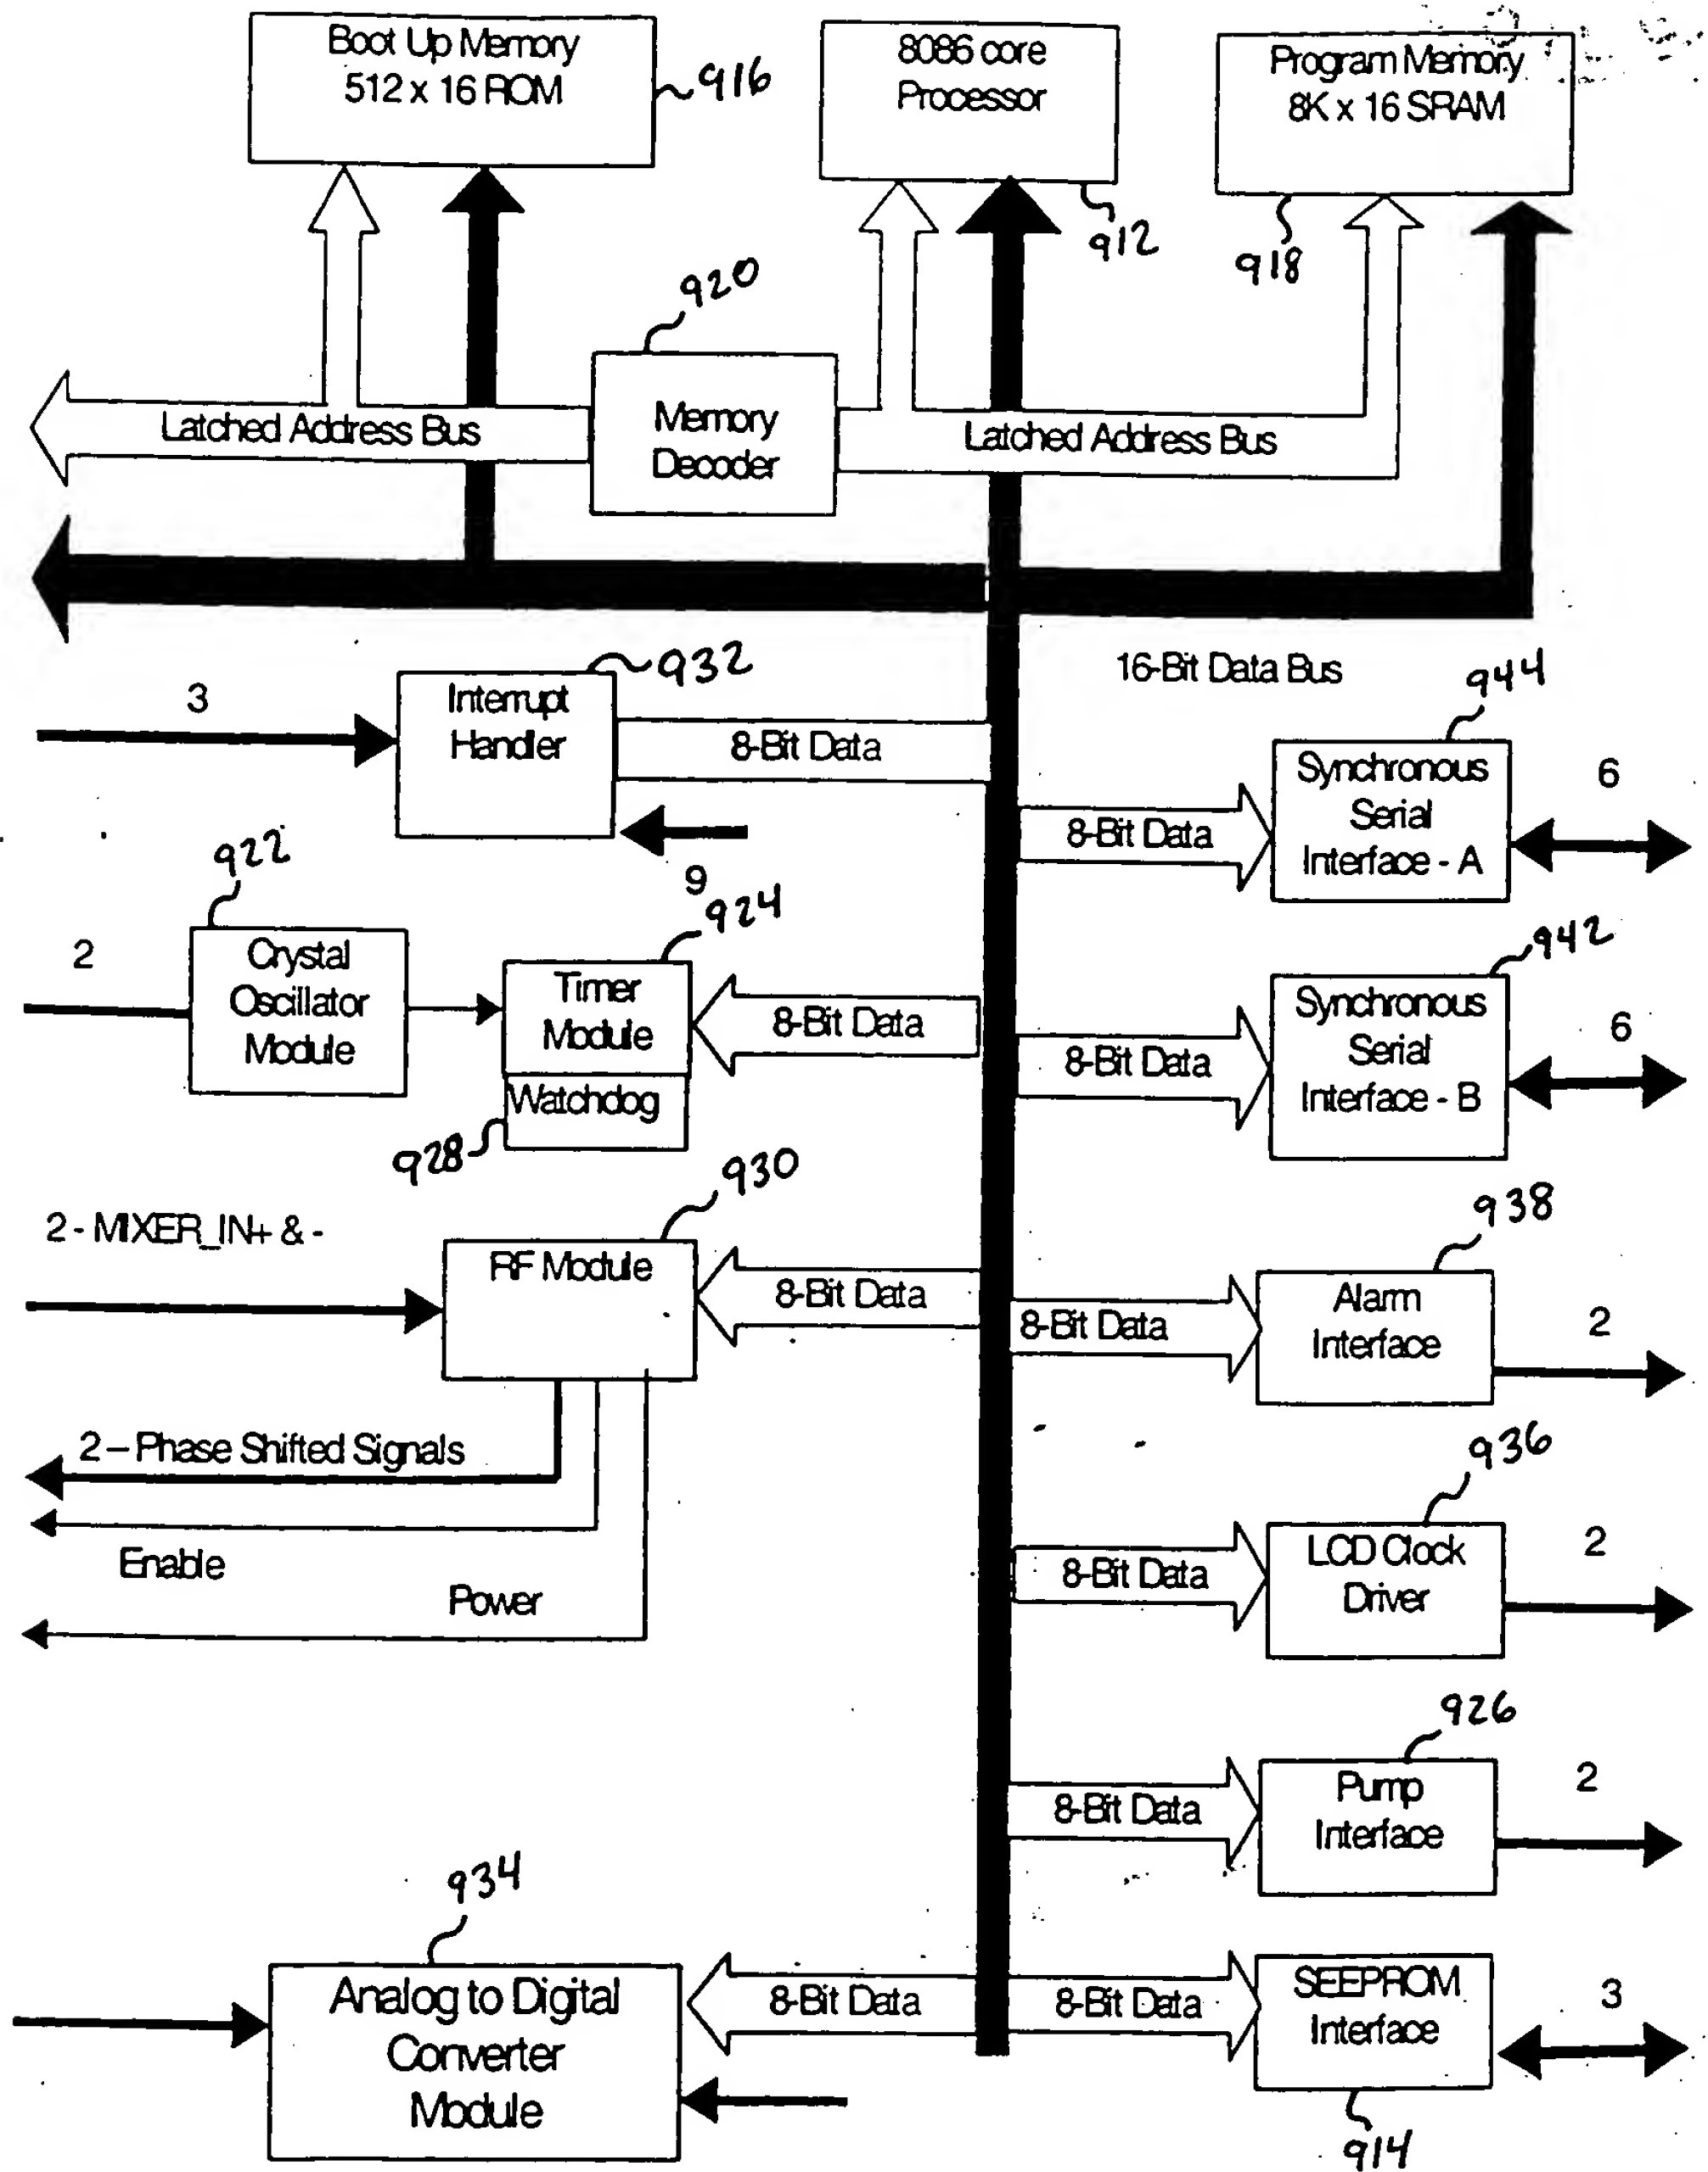


Figure 6

0576196-080901



# Main Menu


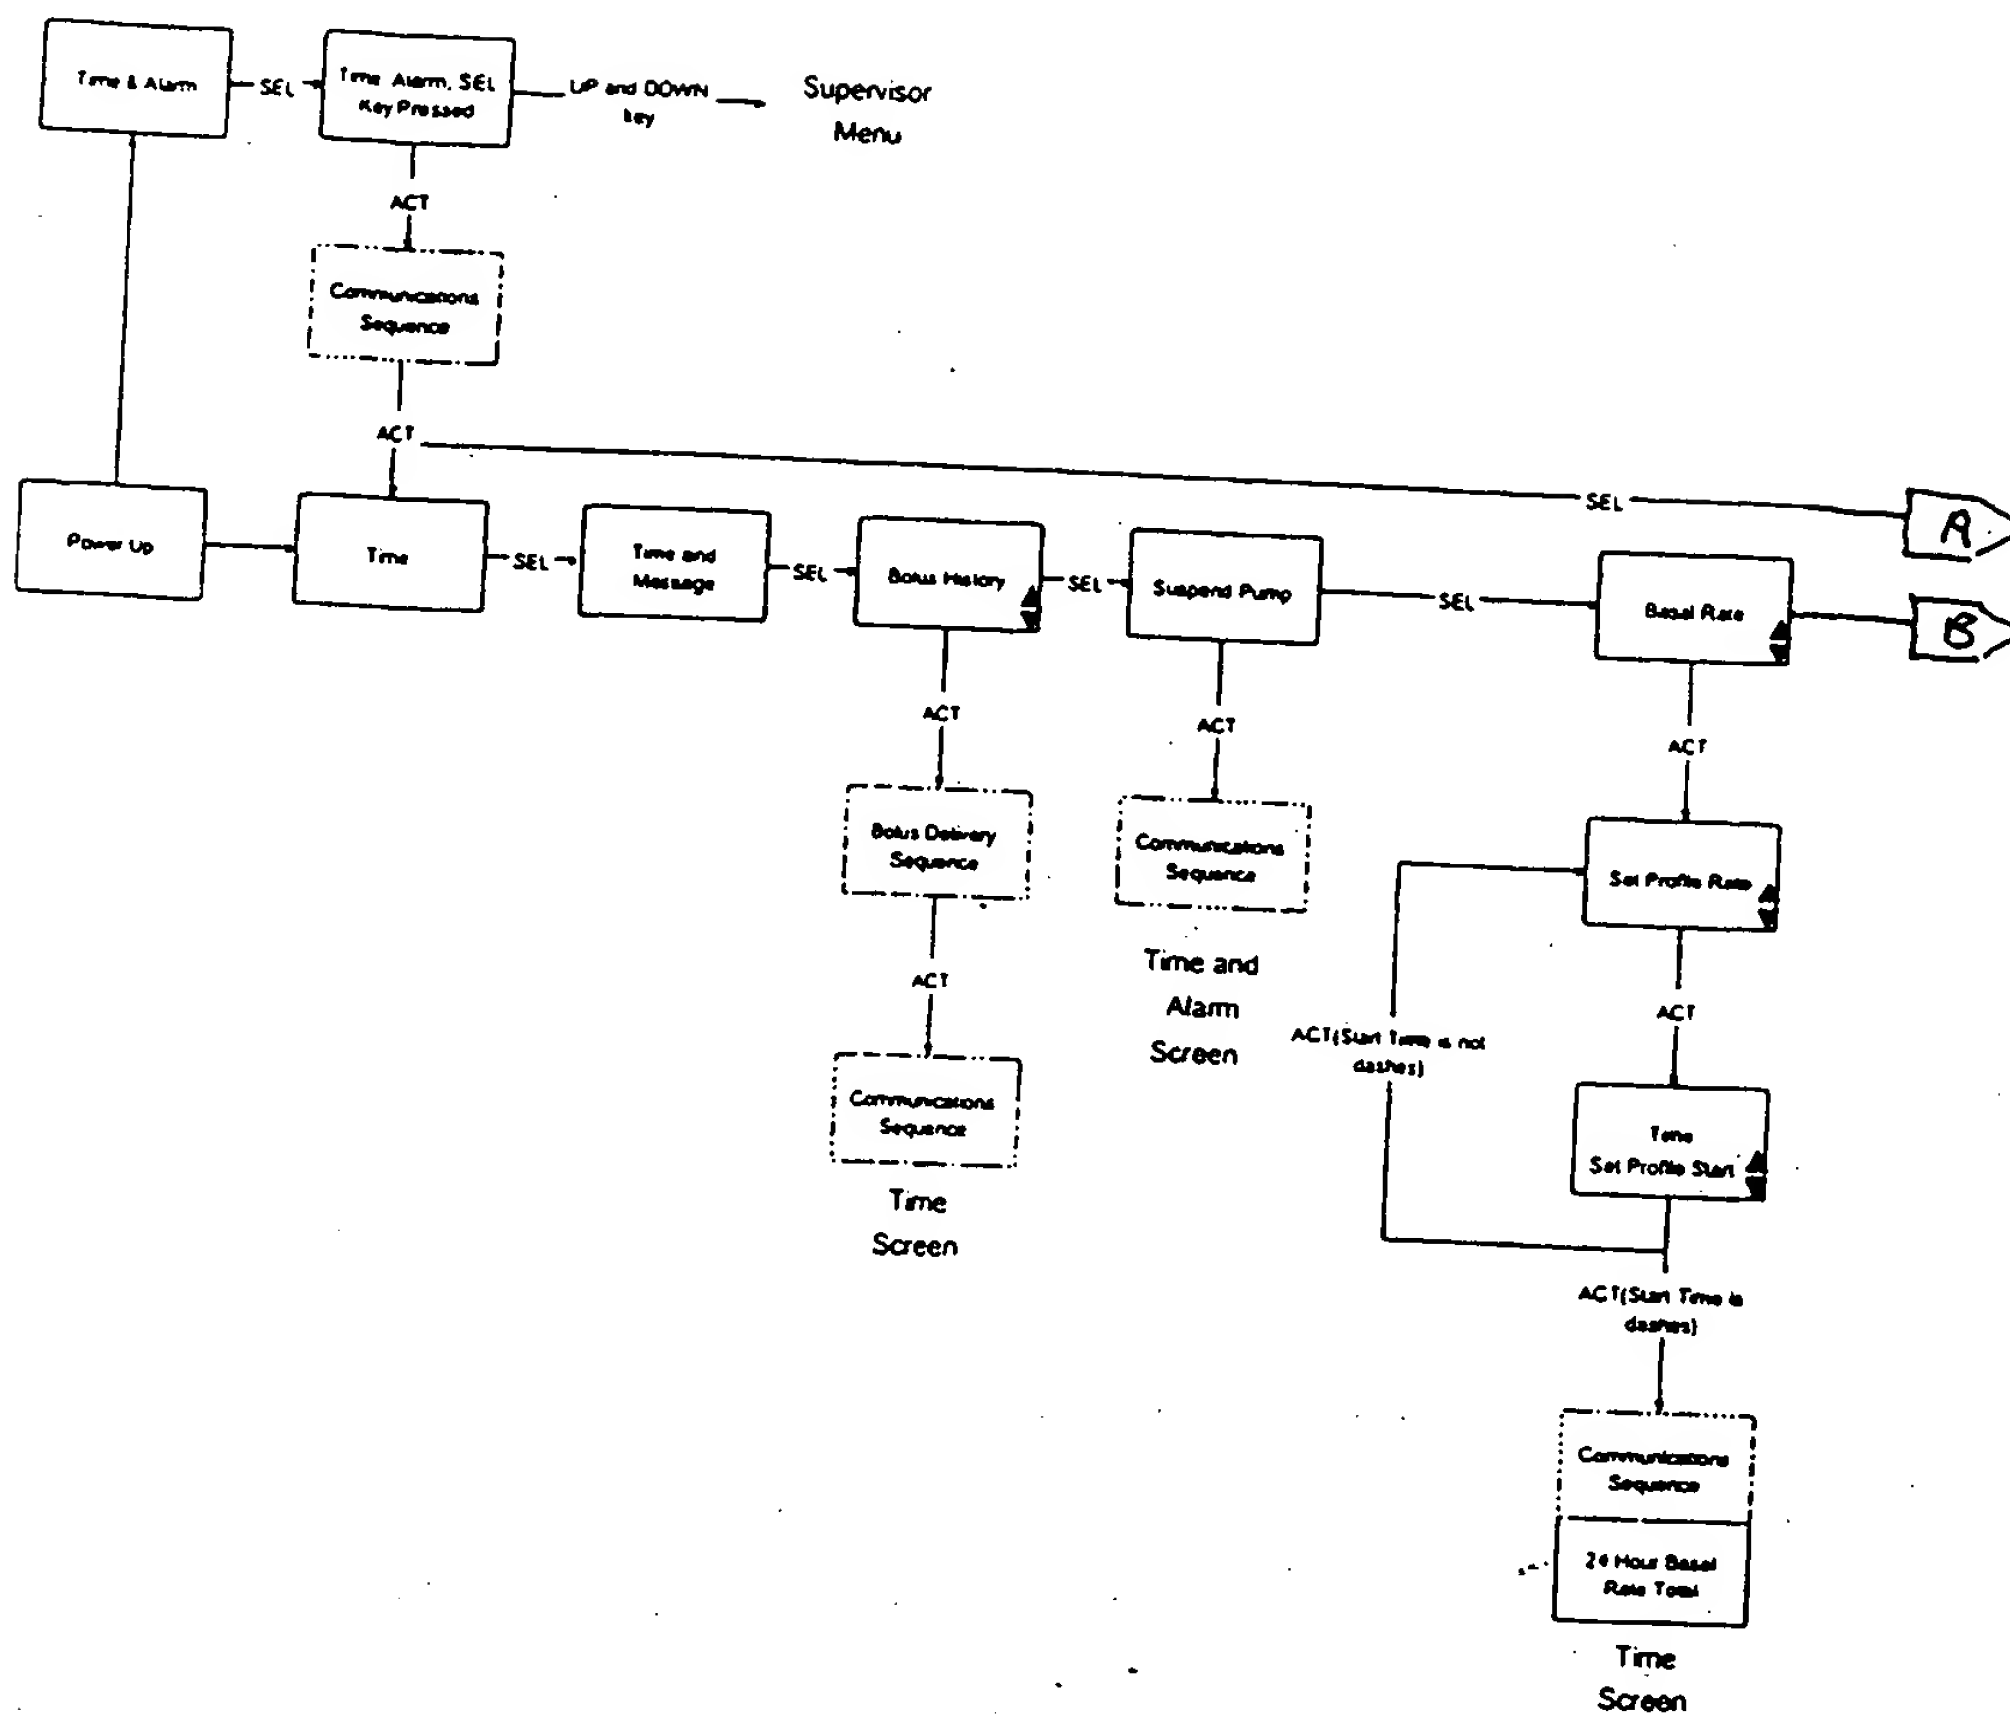


FIGURE 7a





09762195-080304

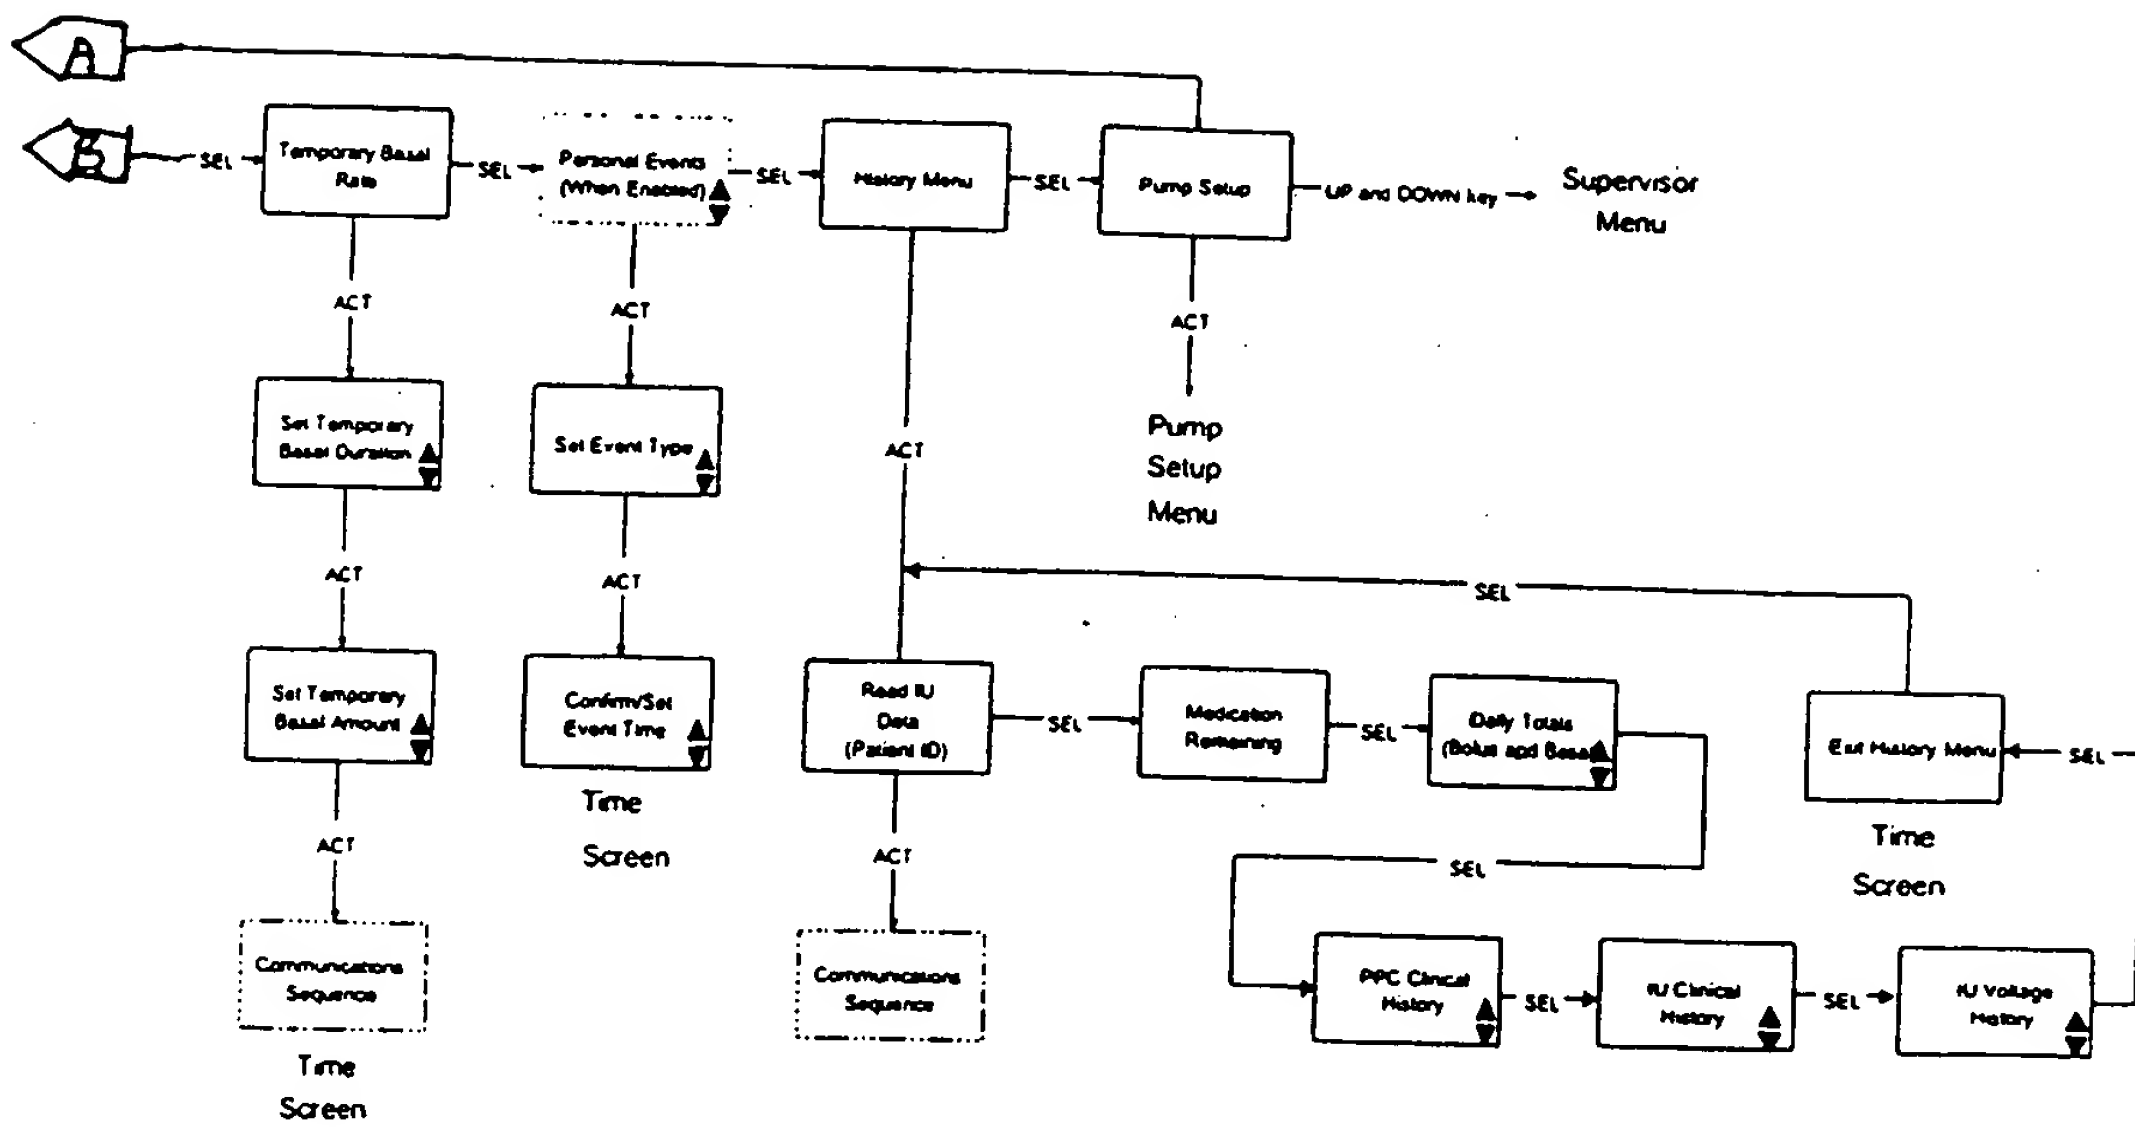

If the Communications Sequence on the History Menu is successful, the next screen in the menu shall be displayed.

FIGURE 7b



# Setup Menus

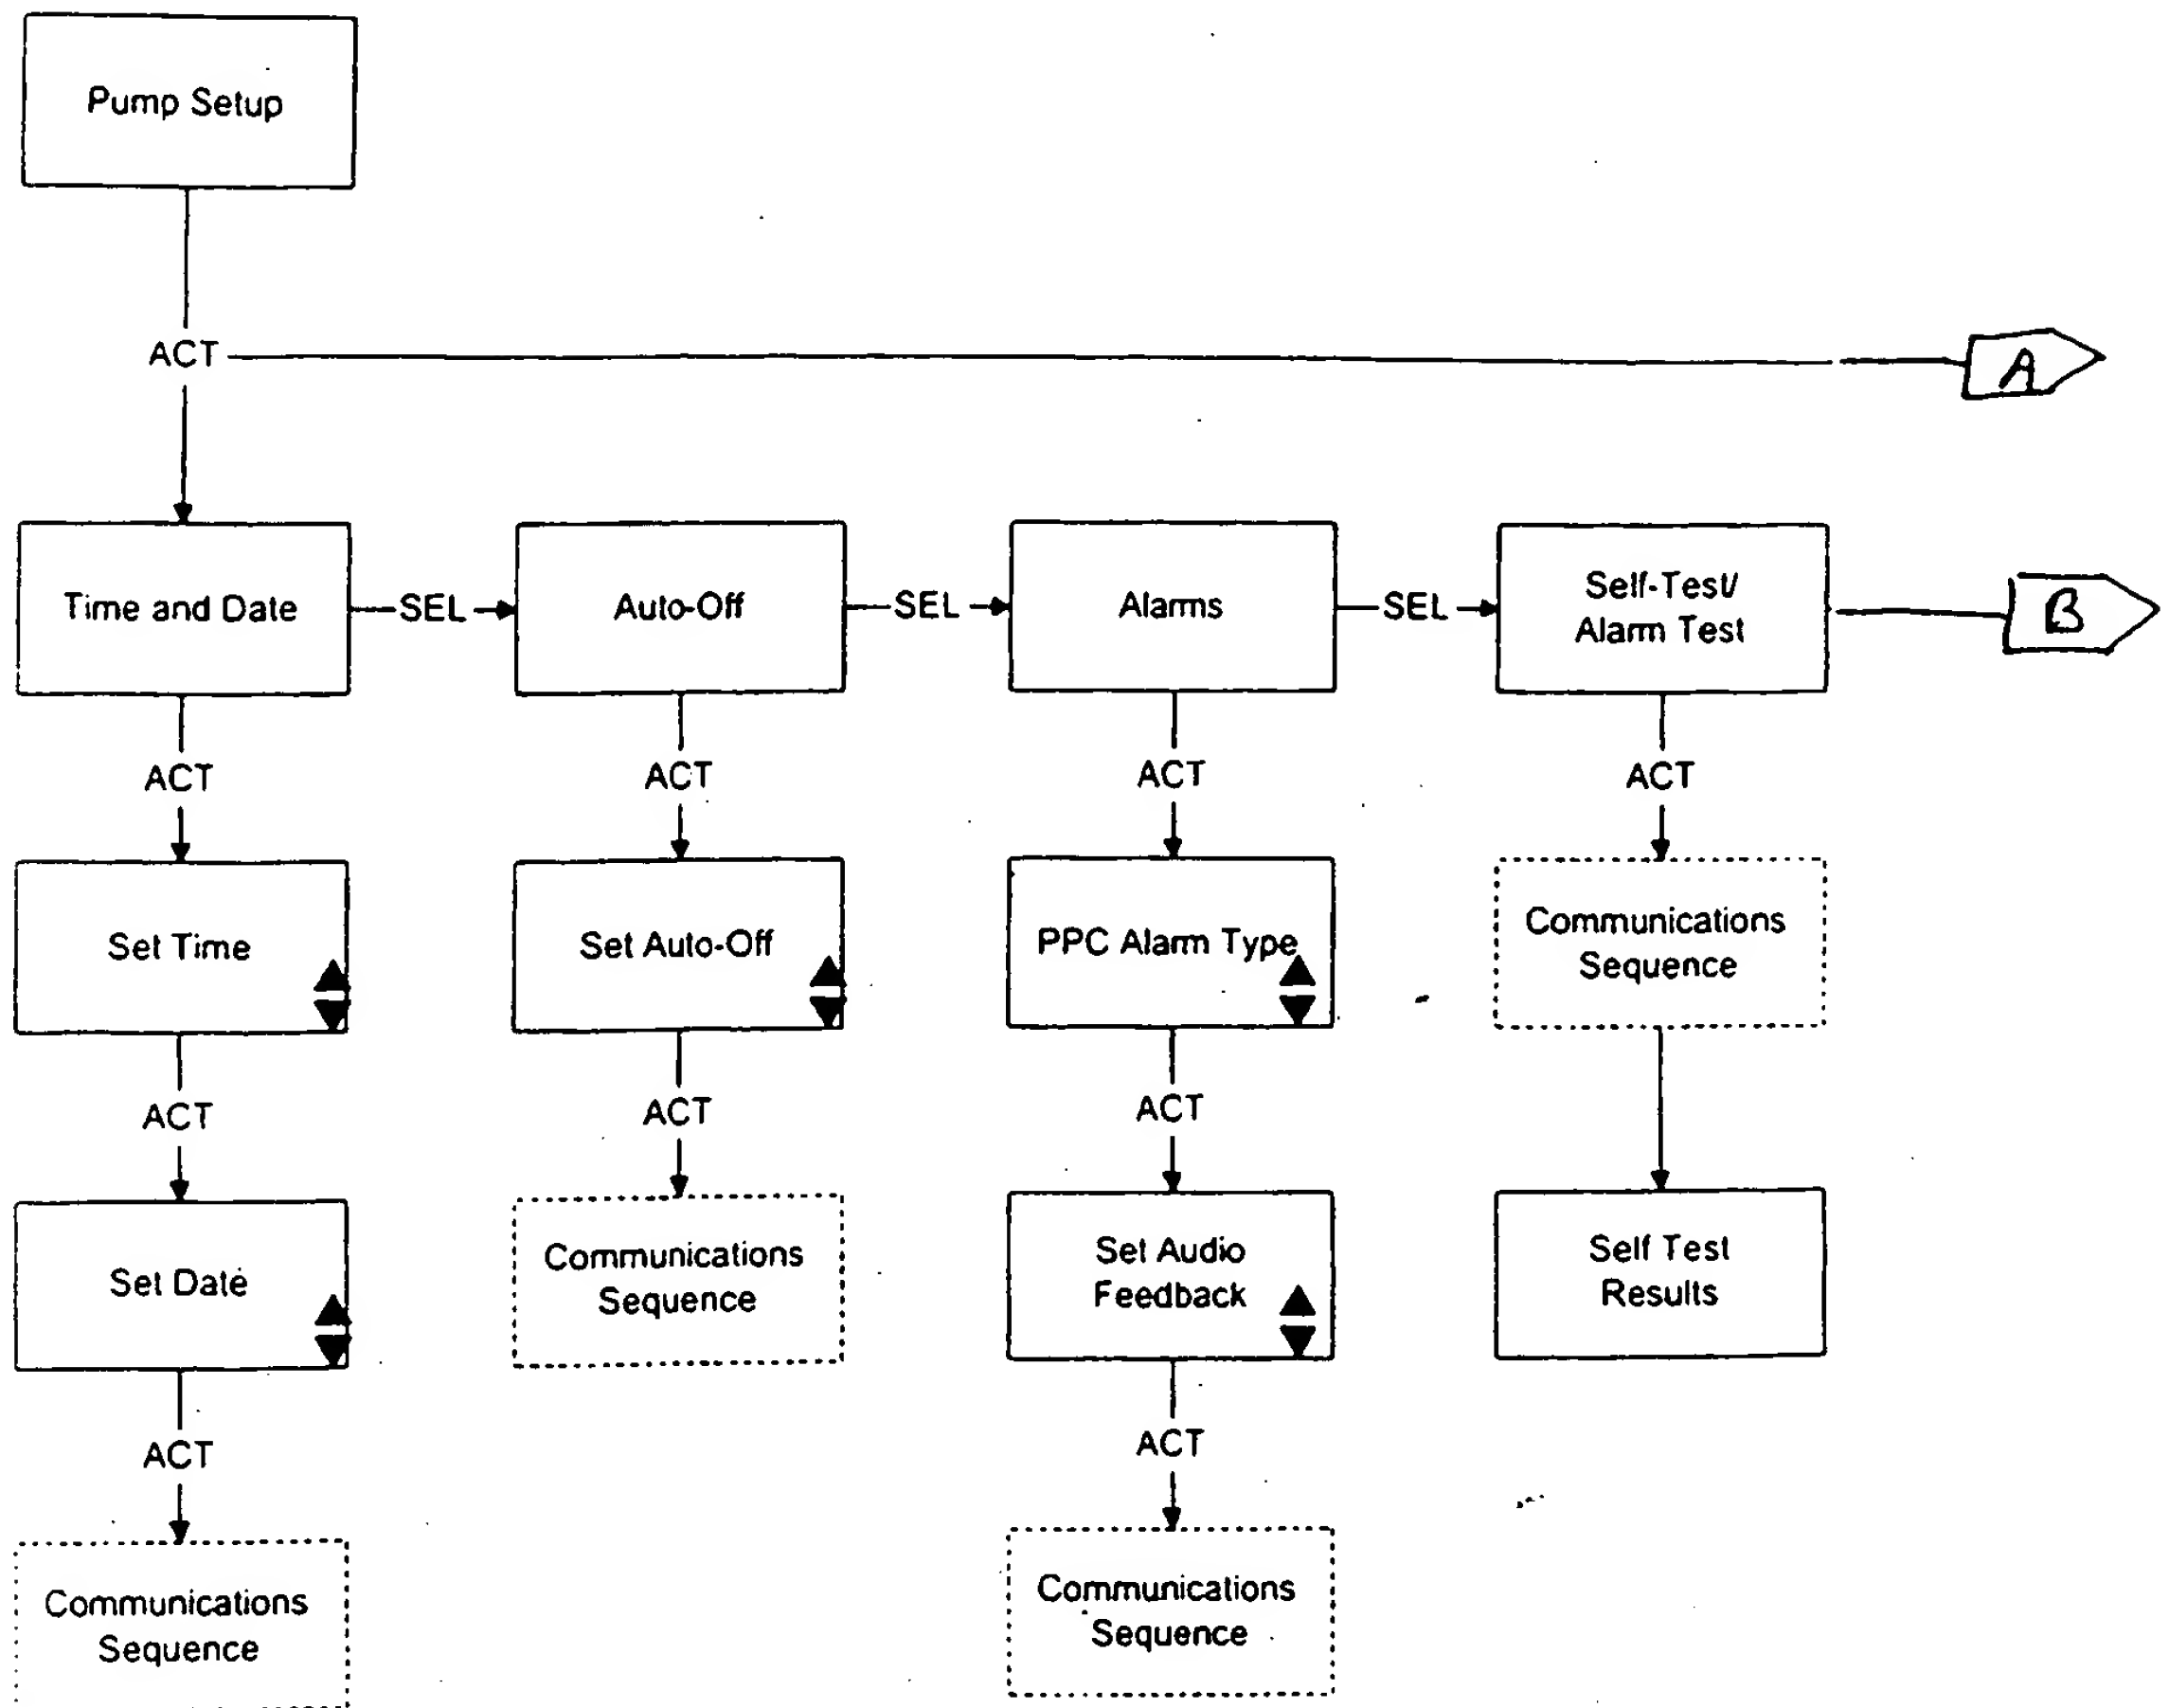


FIGURE 8a


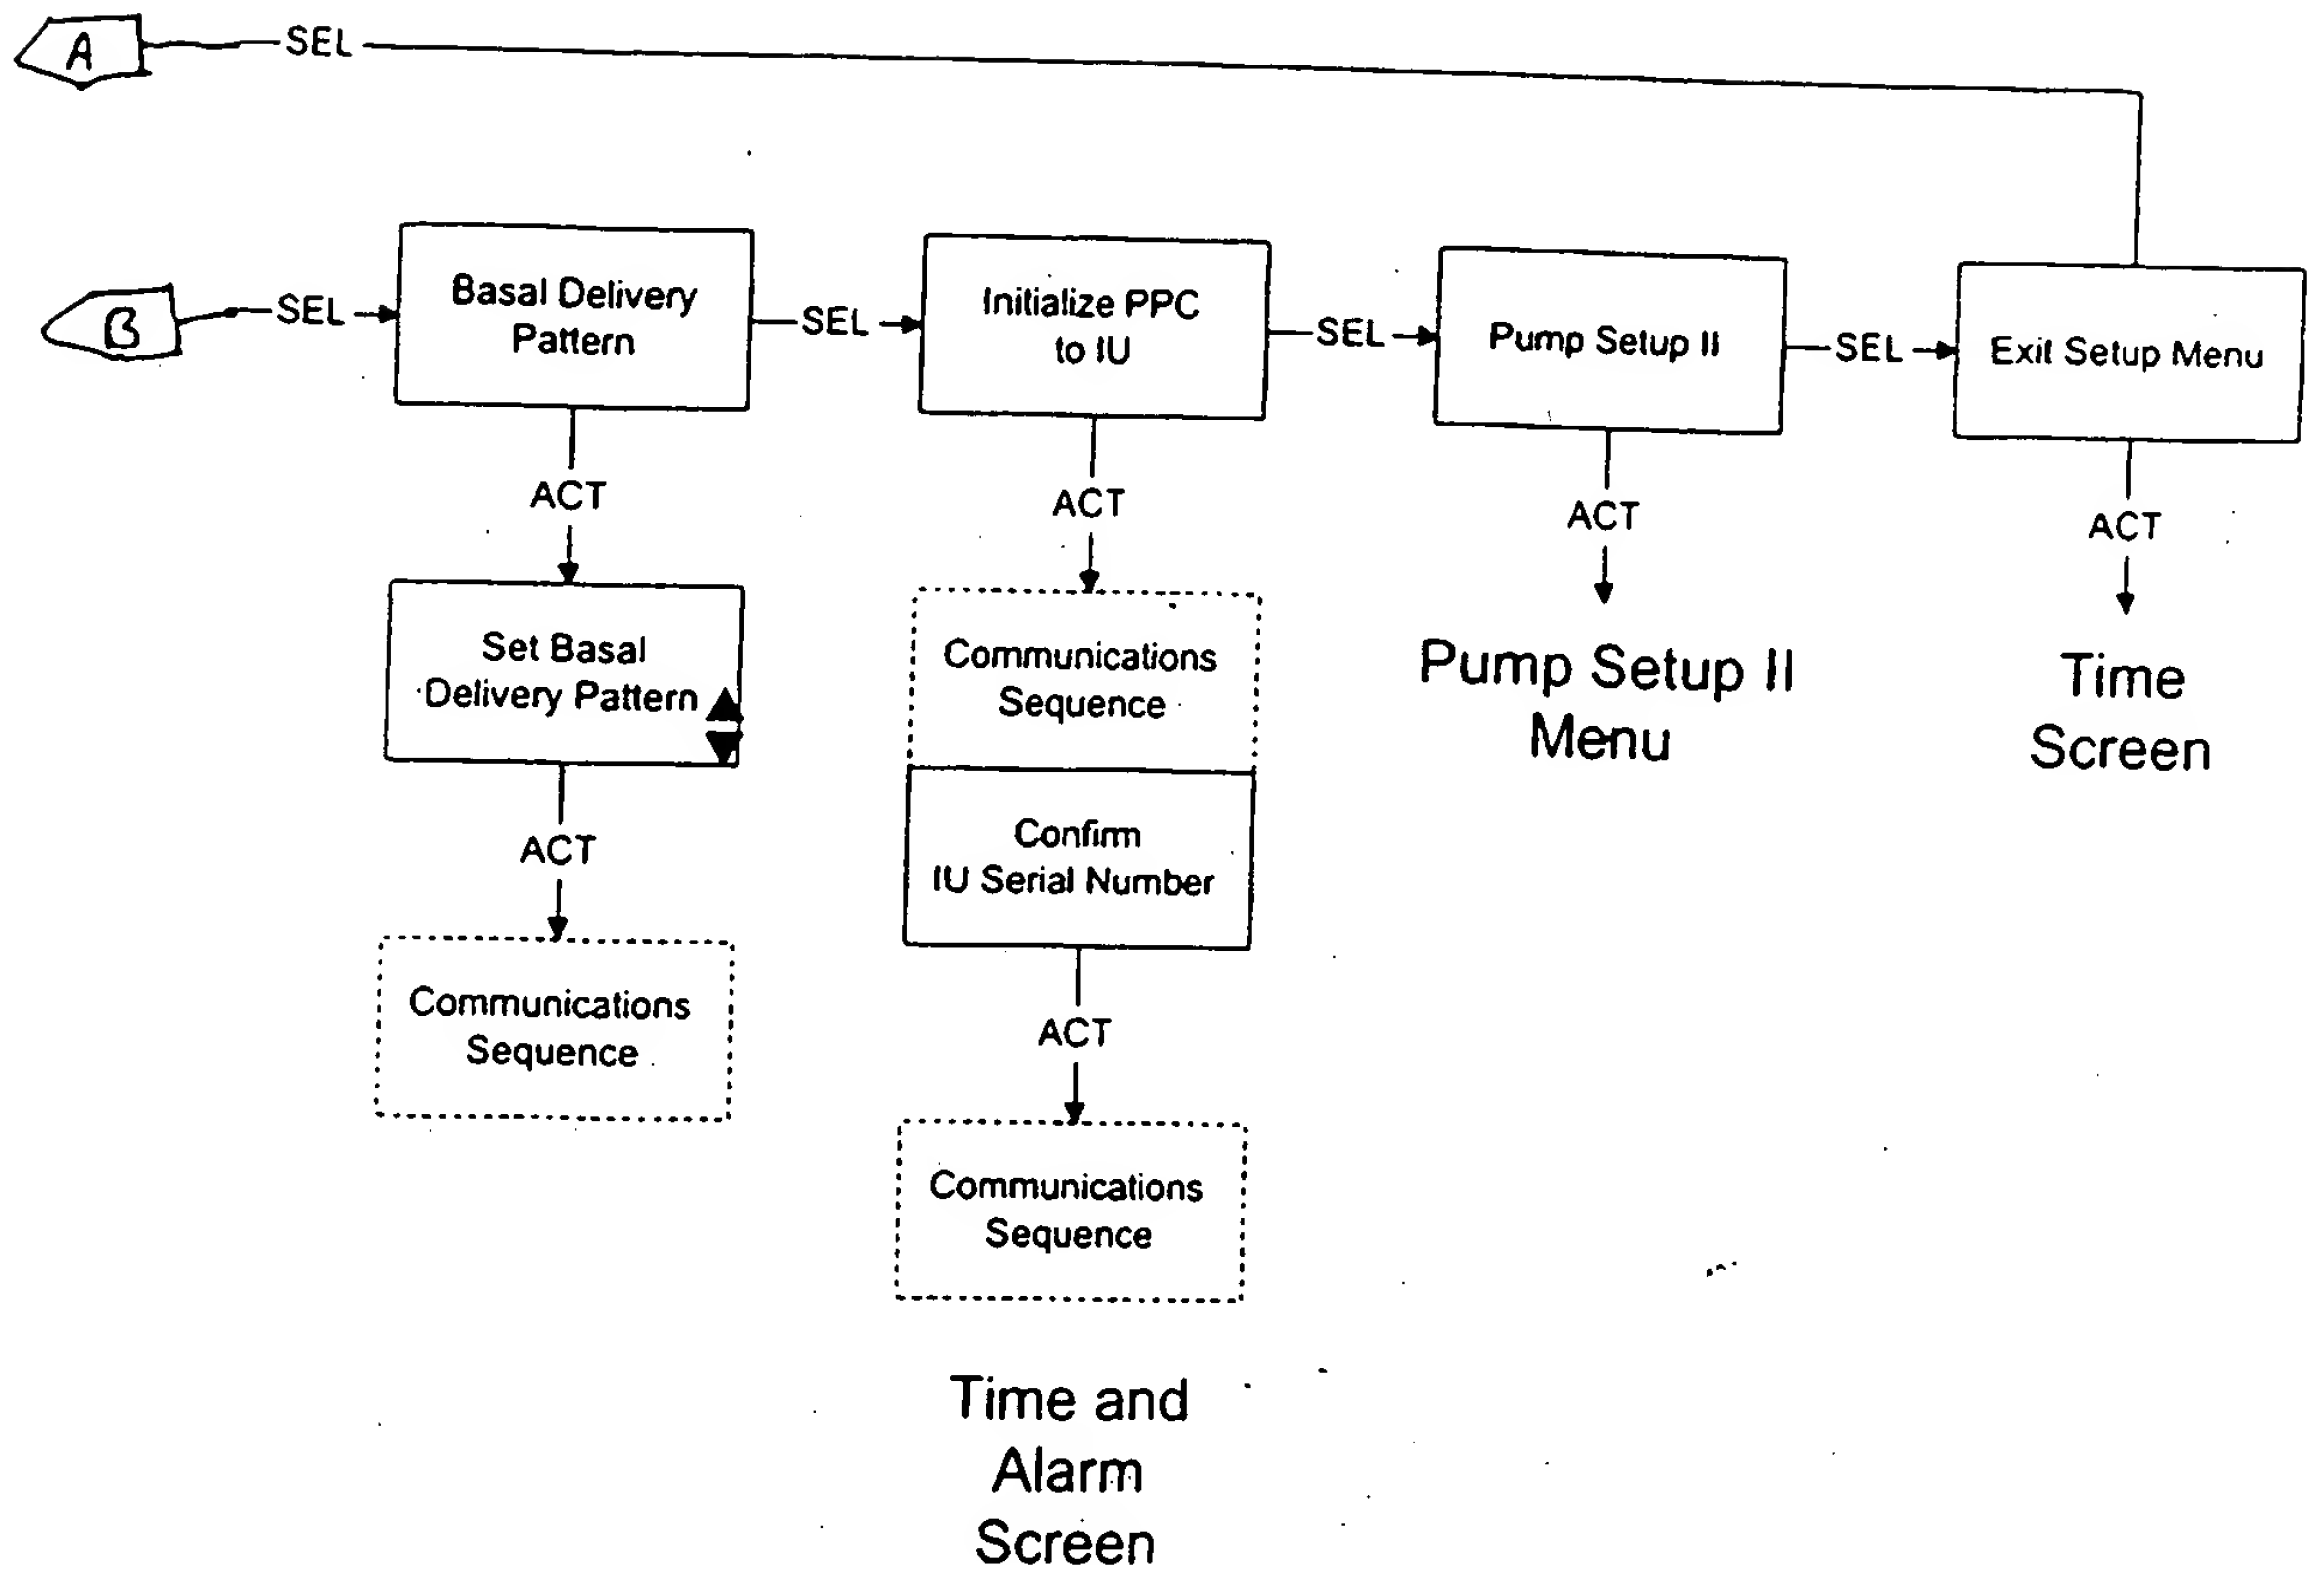


FIGURE 8b

0 1 2 3 4 5 6 7 8 9

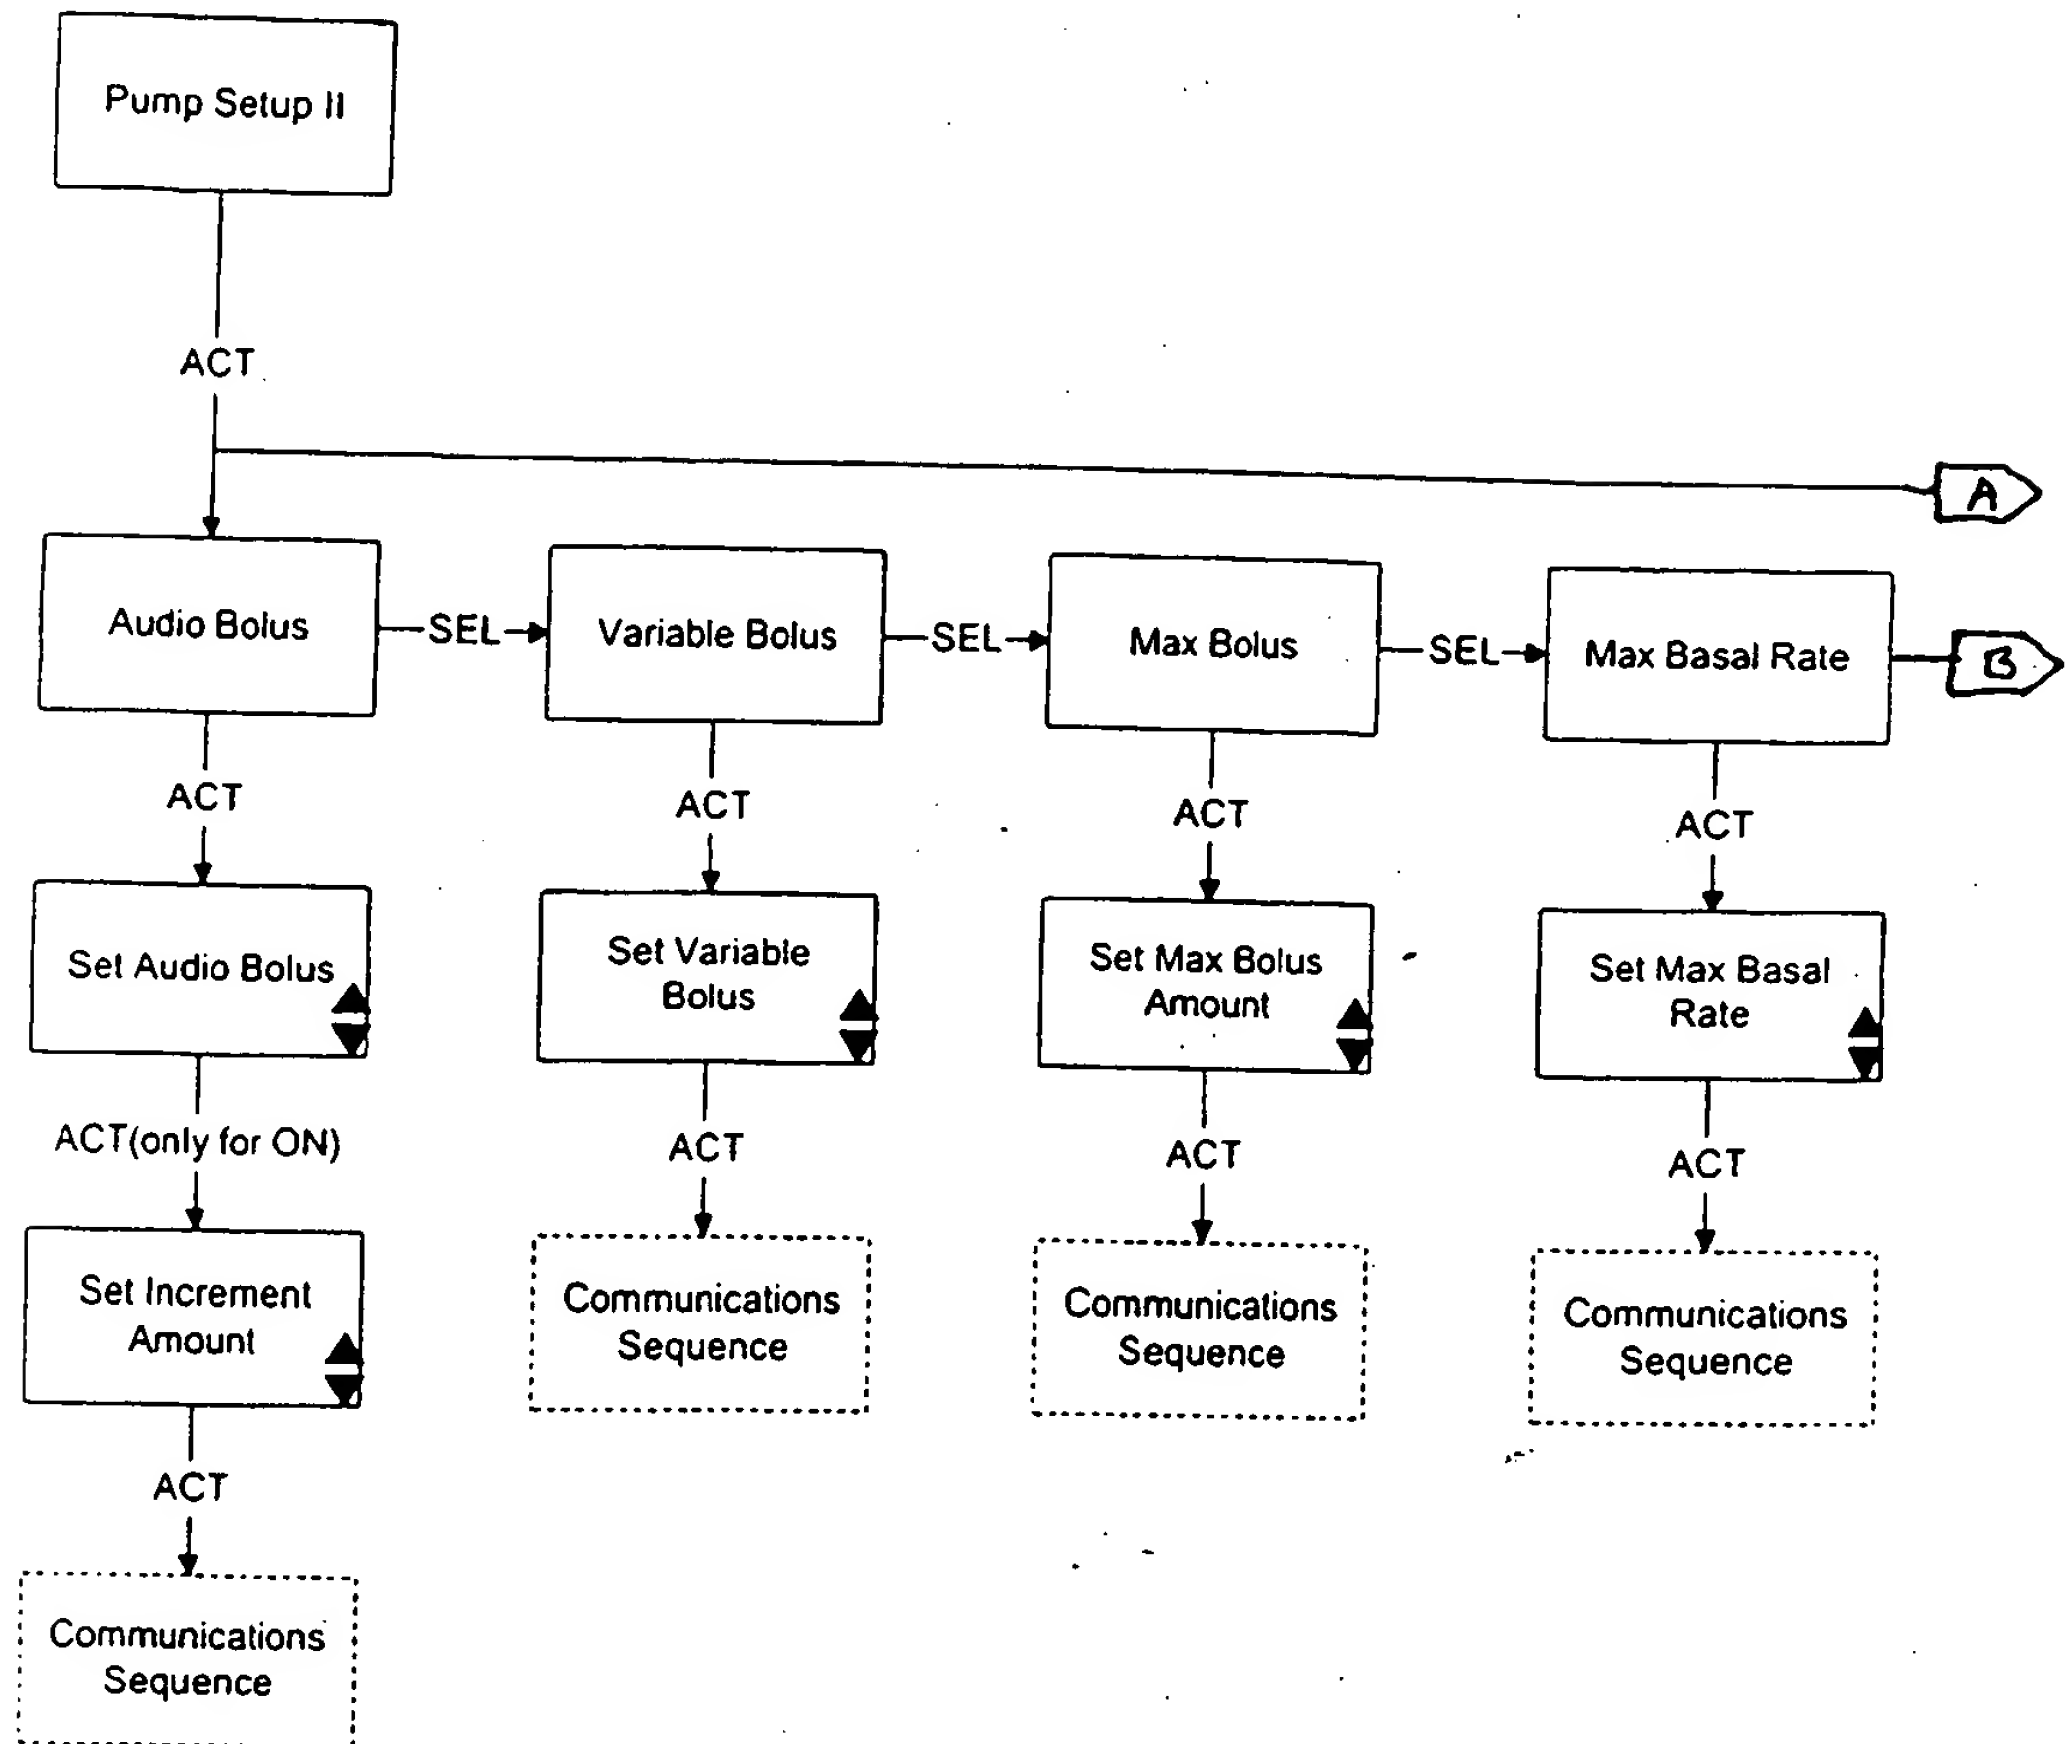

If the Communication Sequence is successful, the next screen in the menu shall be displayed.

FIGURE 9a


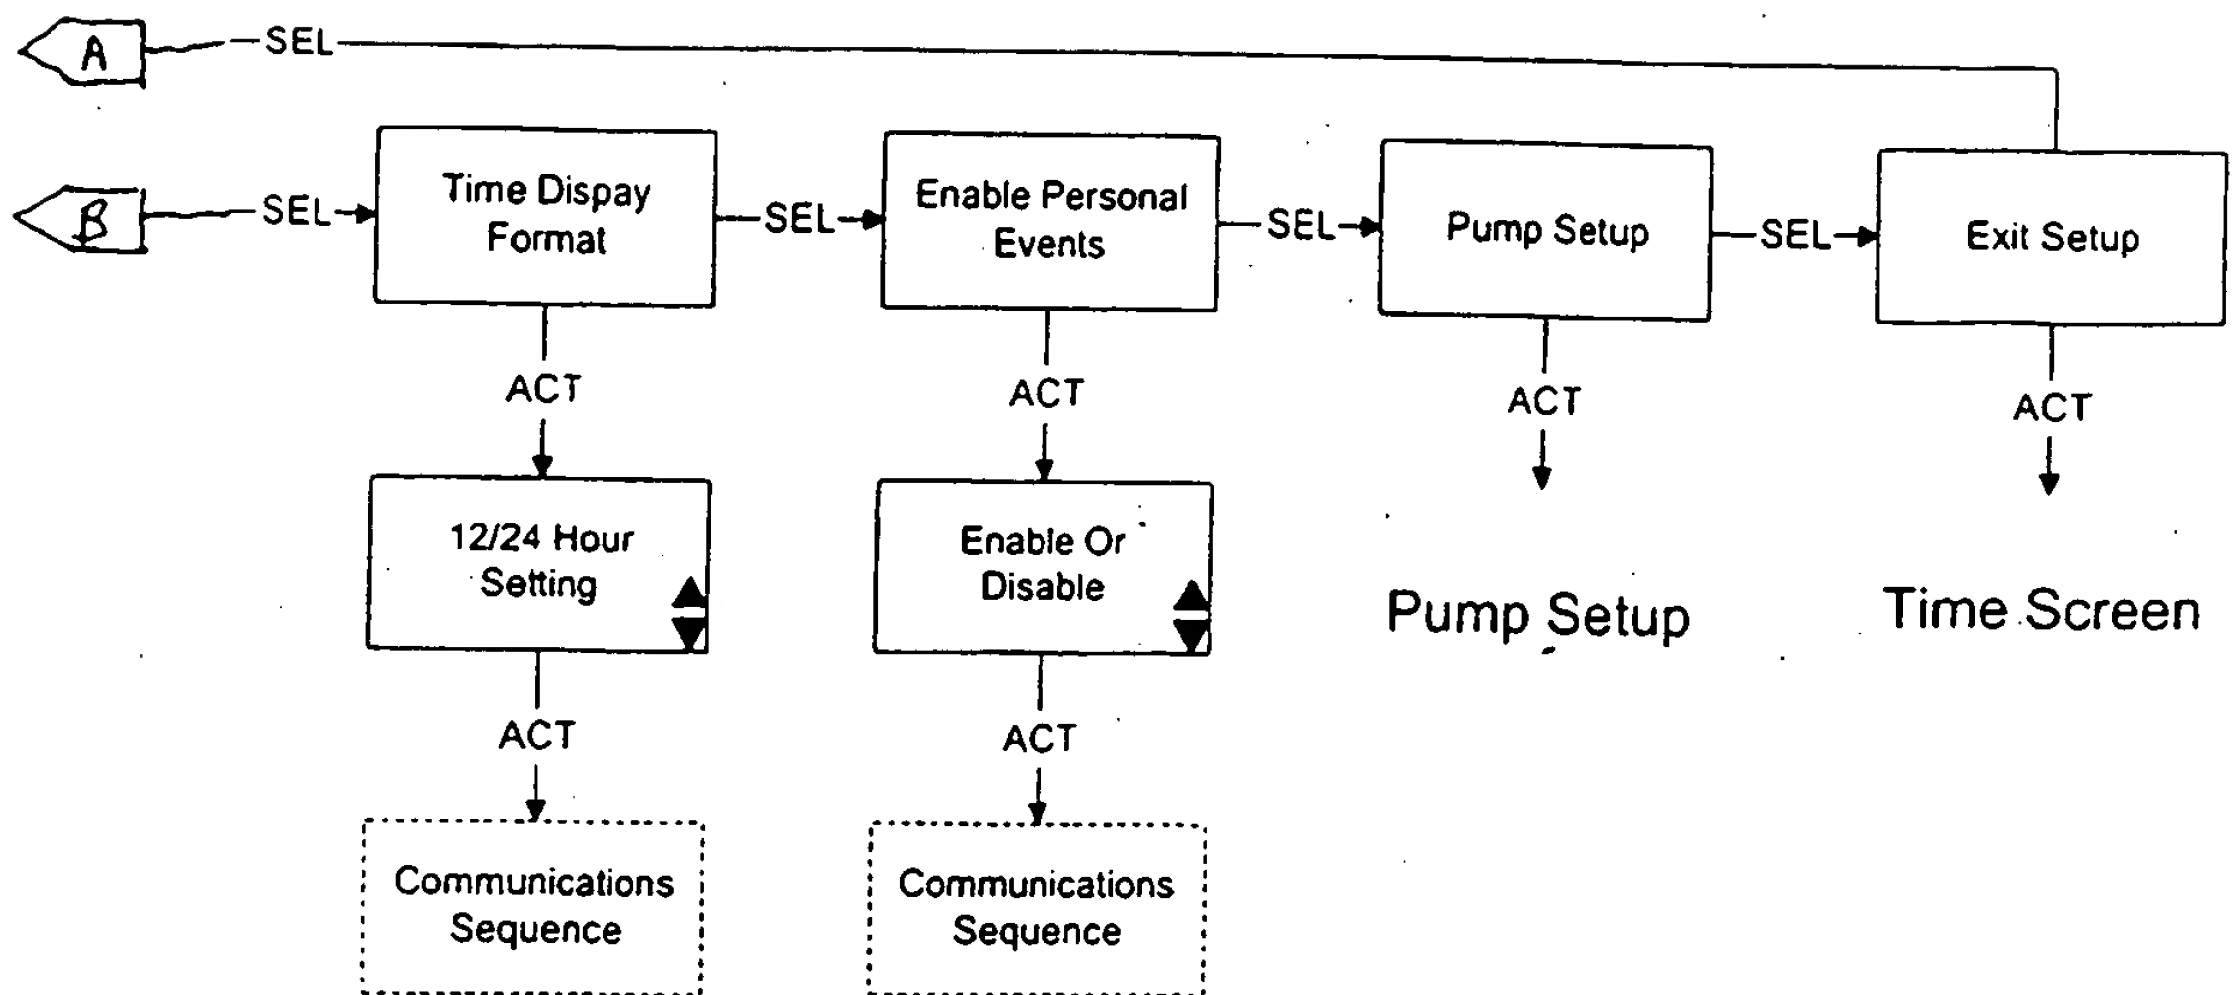


FIGURE 9b

0976196-080901  
T060901 95T89260



# Supervisor Menu

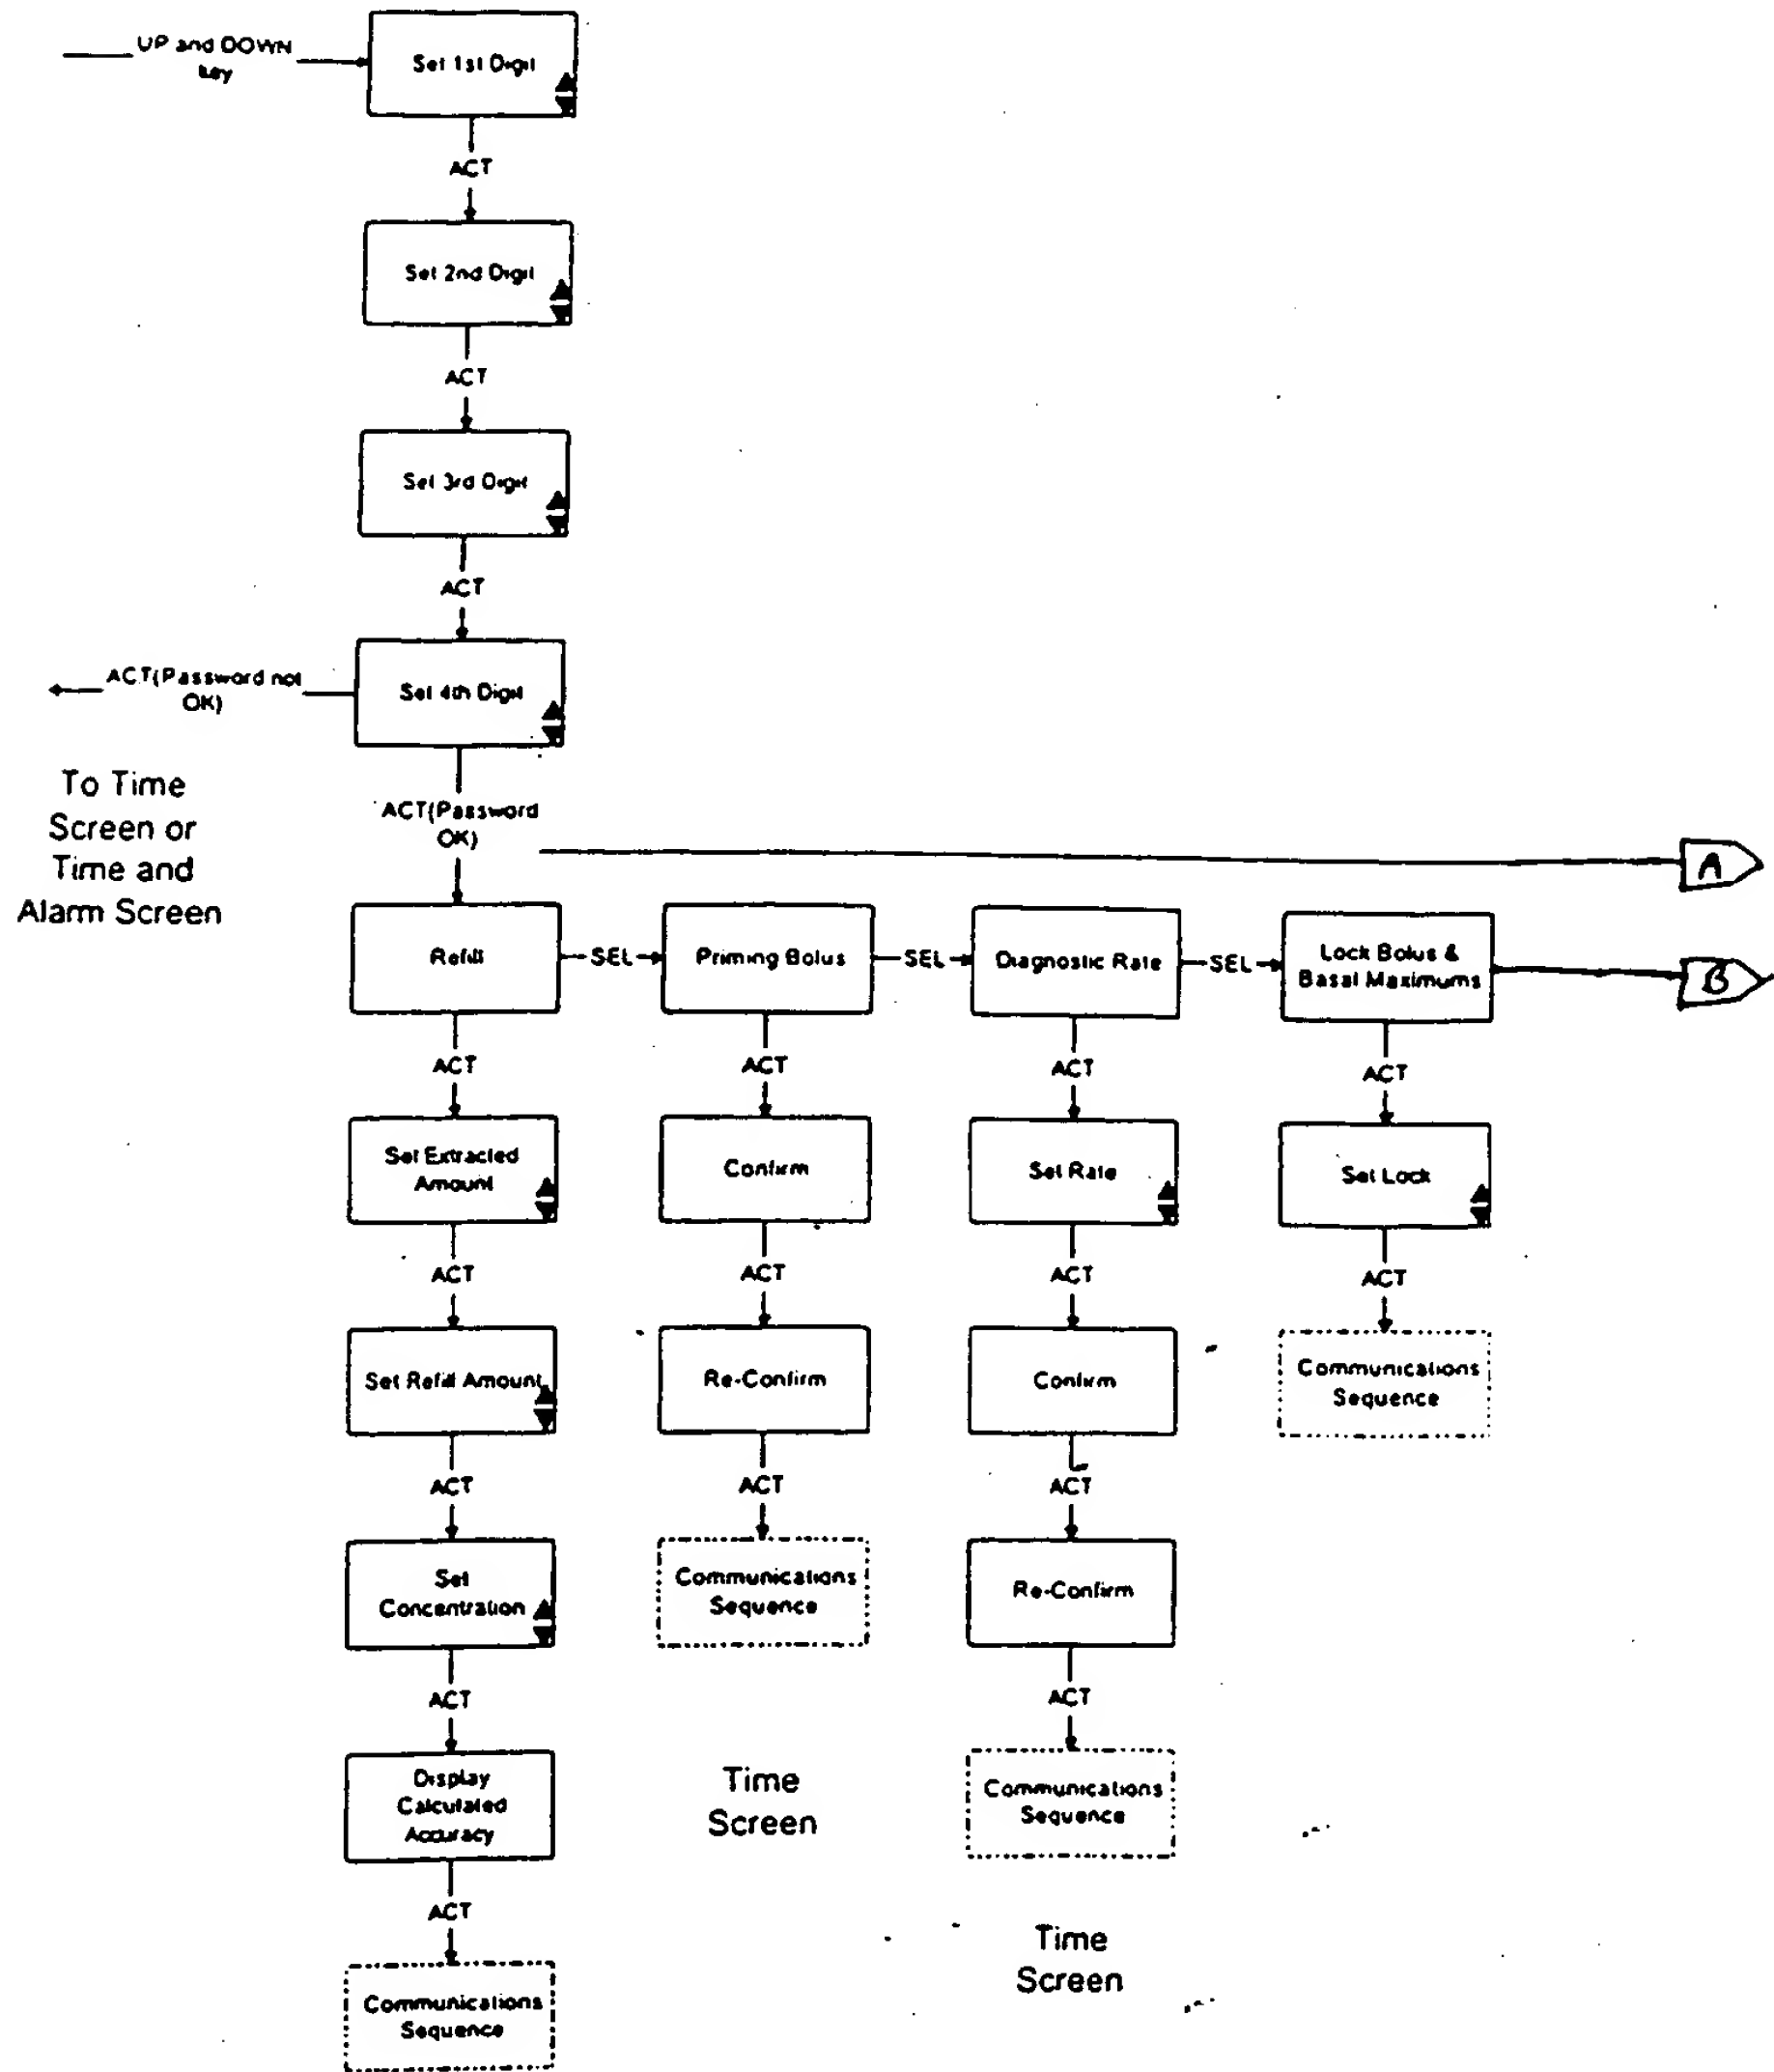

Unless otherwise shown, the screen that follows the Communications Sequence, shall be the next screen on the menu

FIGURE 10a

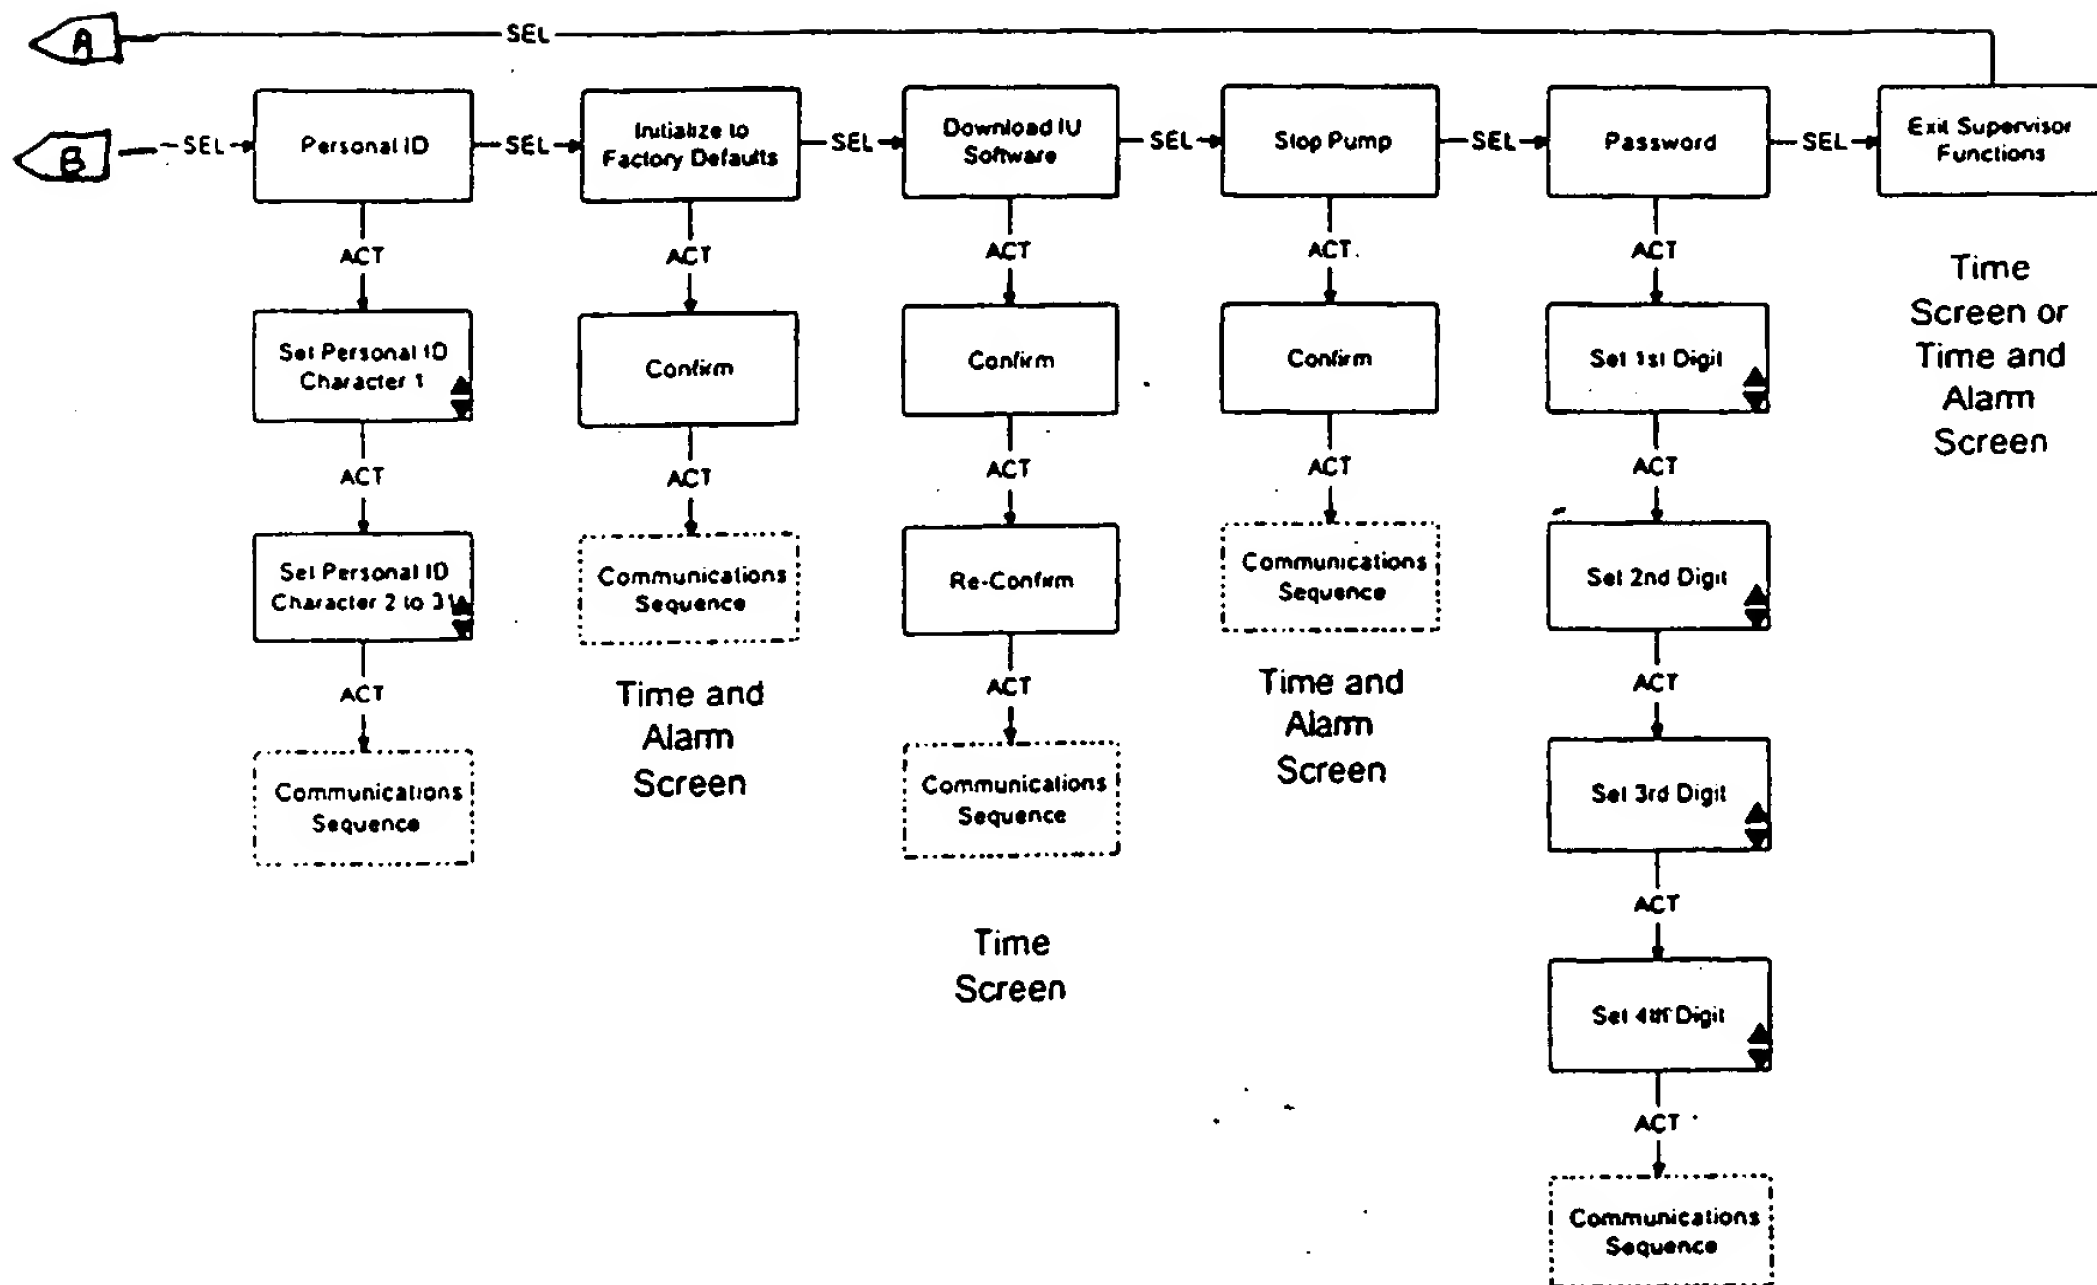


FIGURE 10b



### Communications Sequence

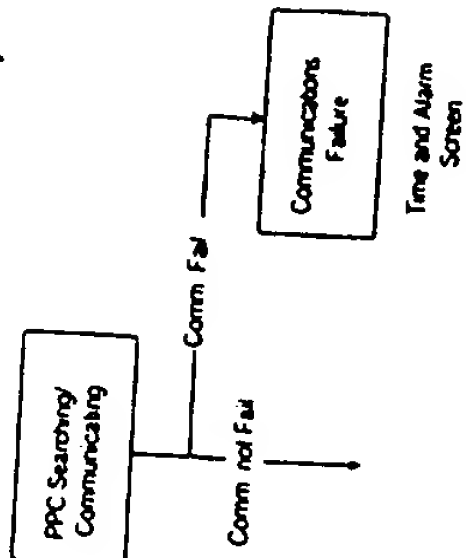


FIGURE 12

## Sequences

### Bolus Delivery Sequence

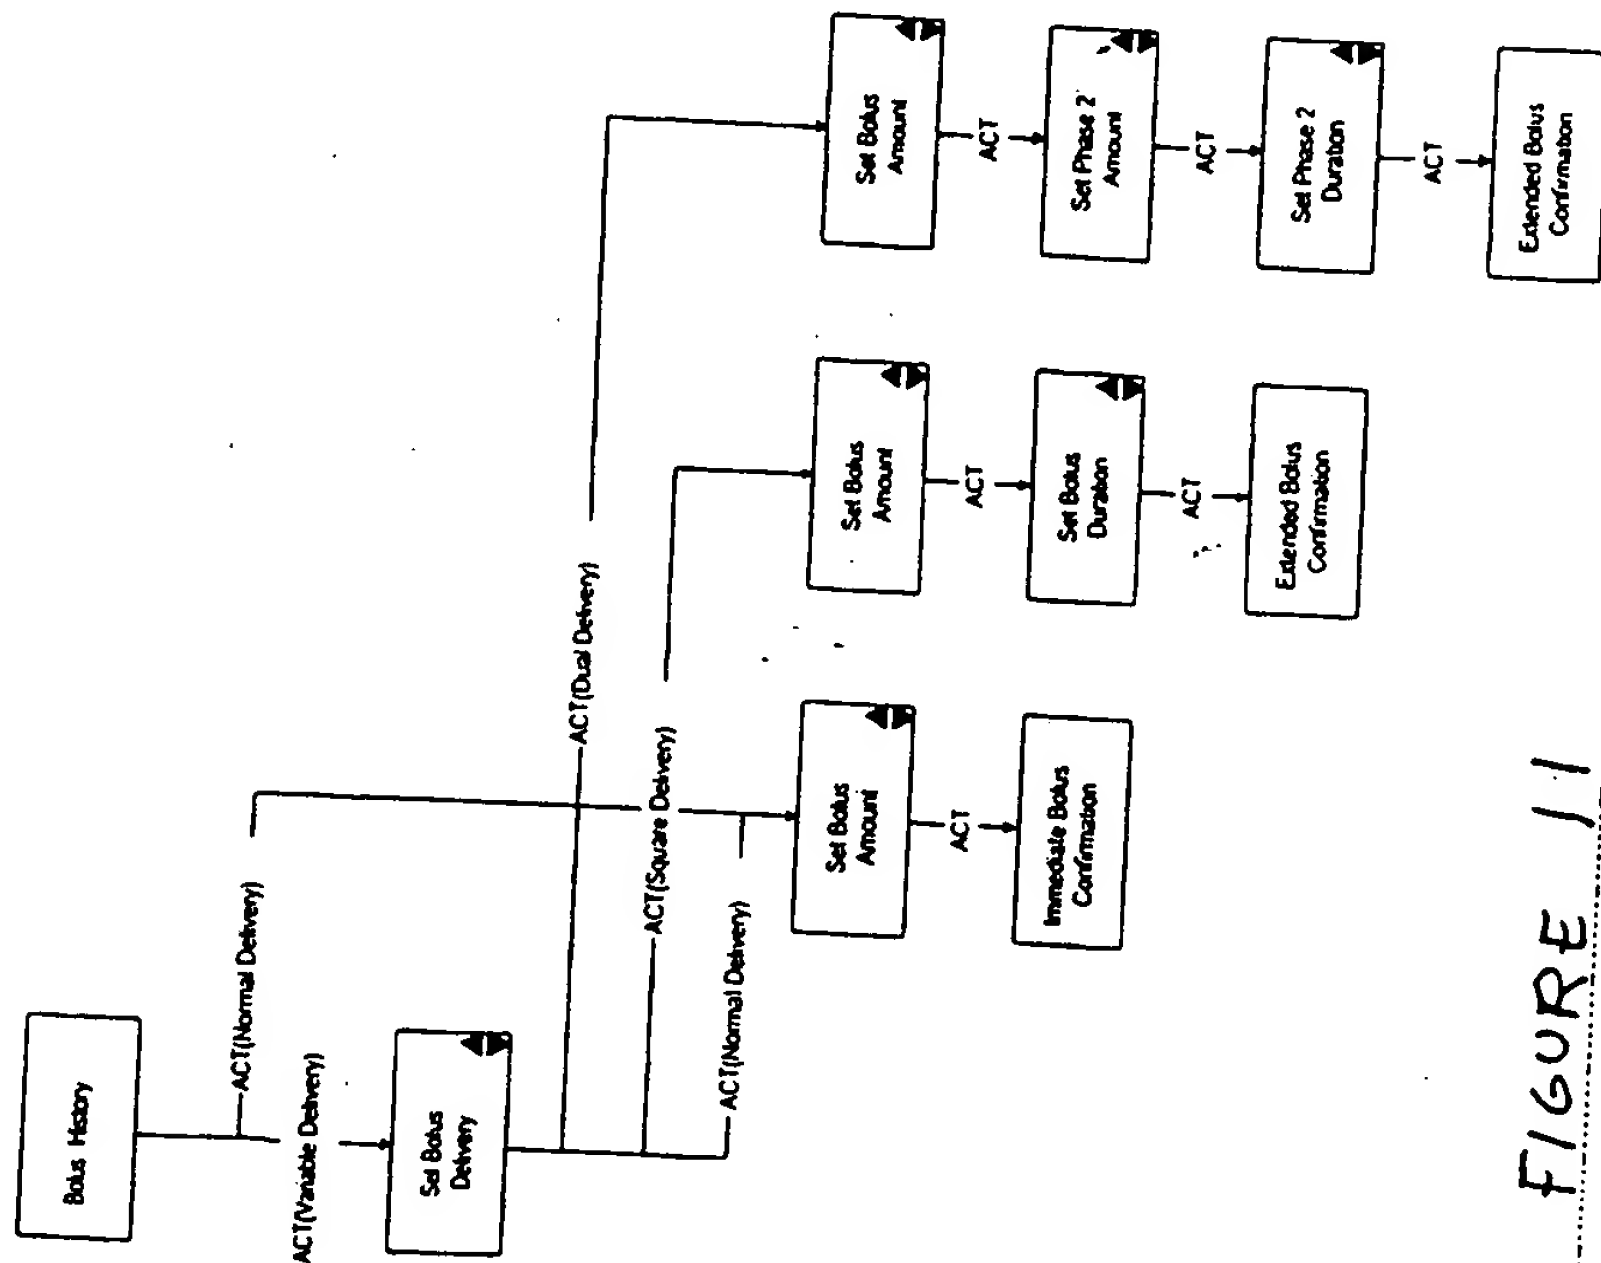


FIGURE 11